



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan
Micron Test Report

Sugartown Farms/Timm & Helen Herman
6277 Sugartown Rd
Ellicottville NY 14731 USA

08/04/17

Test No: 947876


Animal and Sample Description

Animal Name: Black Escapade
Breed: Alpaca(Huacaya)
Sex: Male
Color: Black

Animal ID: 35149101
Sample Location: Side
Sample Date: 05/22/17
Age: 09/19/16

Laboratory Data

Mean Fiber Diameter: 19.2 microns
Standard Deviation: 3.9 microns
Coefficient of Variation: 20.4 %
Fibers Greater Than 30 microns: 1.2 %

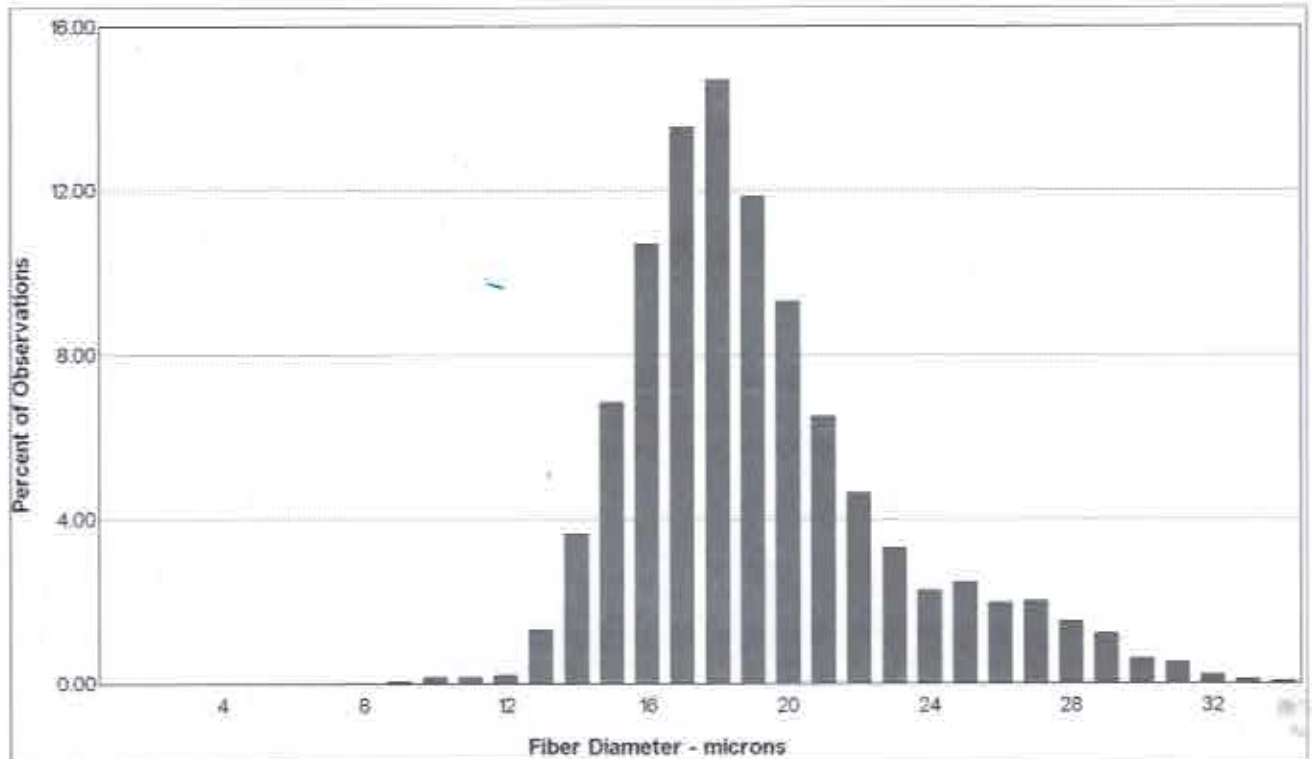

This Test Performed According to I.W.T.O Method 12