



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Ariya Alpacas Inc/Janette Archambault
411 Brill Road RR32
West Bolton QC J0E 2T0 Canada

Date: 02/01/16

Test No: 918350


Animal and Sample Description

Animal Name: Xclipse's Belenis
Breed: Alpaca(Huacaya)
Sex: Male
Color: Beige

Animal ID: 35255123
Sample Location: Side
Sample Date: 01/16/16
Age: 06/10/14

Laboratory Data

Mean Fiber Diameter:	16.0 microns	Fibers Greater Than 30 microns:	0.1 %
Standard Deviation:	3.1 microns	Comfort Factor:	99.9 %
Coefficient of Variation:	19.2 %	Mean Curvature:	42.0 deg/mm
Spin Fineness:	15.3 microns	SD Curvature:	23.0 deg/mm

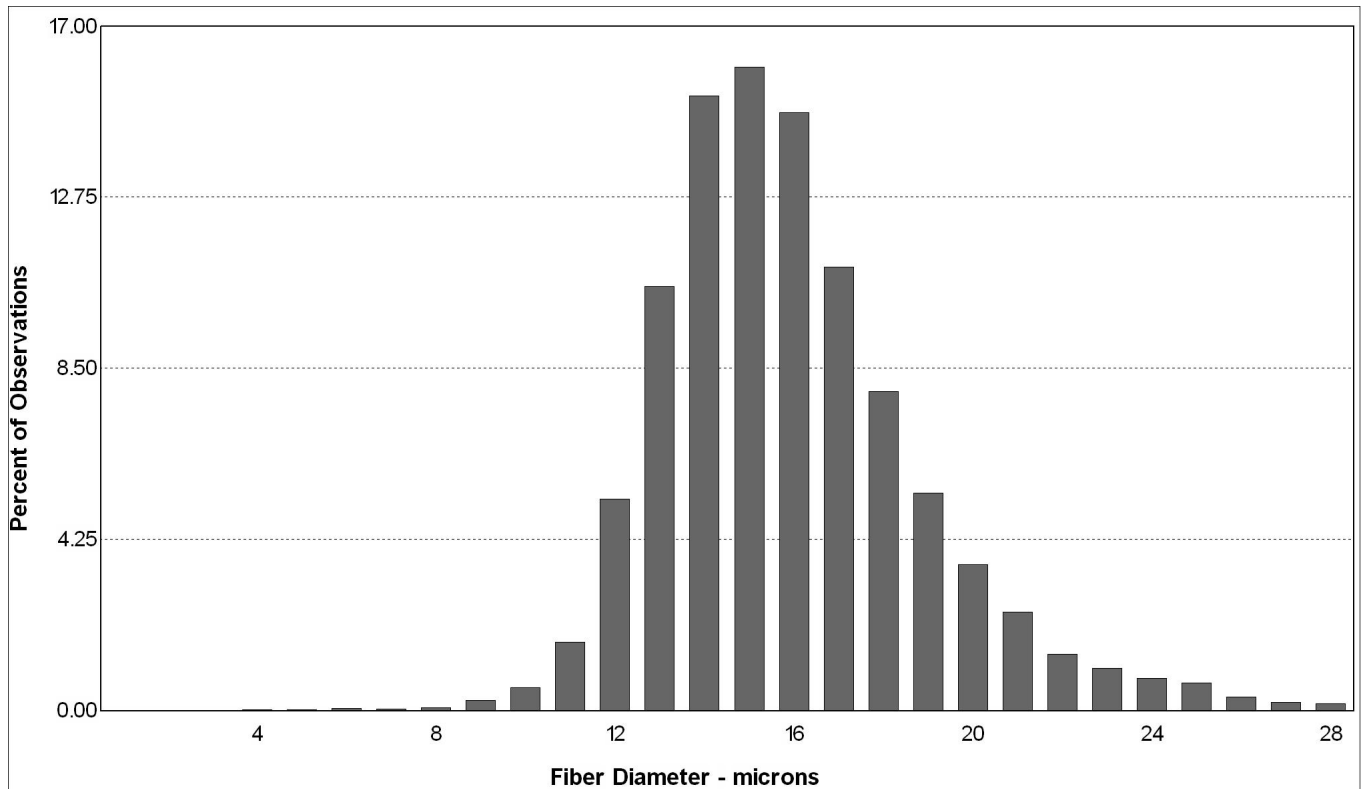

This Test Performed According to I.W.T.O Method 47