



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Ariya Alpacas Inc/Janette Archambault
411 Chemin De Brill Road, RR32
Bolton Ouest QC J0E 2T0 Canada

Date: 08/05/18

Test No: 965444


Animal and Sample Description

Animal Name: Kamaaina Kailani
Breed: Alpaca(Huacaya)
Sex: Female
Color: XXXXX

Animal ID: 32354256
Sample Location: Side
Sample Date: 05/28/18
Age: 06/11/13

Laboratory Data

Mean Fiber Diameter:	20.5 microns	Fibers Greater Than 30 microns:	2.7 %
Standard Deviation:	4.3 microns	Comfort Factor:	97.3 %
Coefficient of Variation:	21.0 %	Mean Curvature:	43.7 deg/mm
Spin Fineness:	19.9 microns	SD Curvature:	33.1 deg/mm

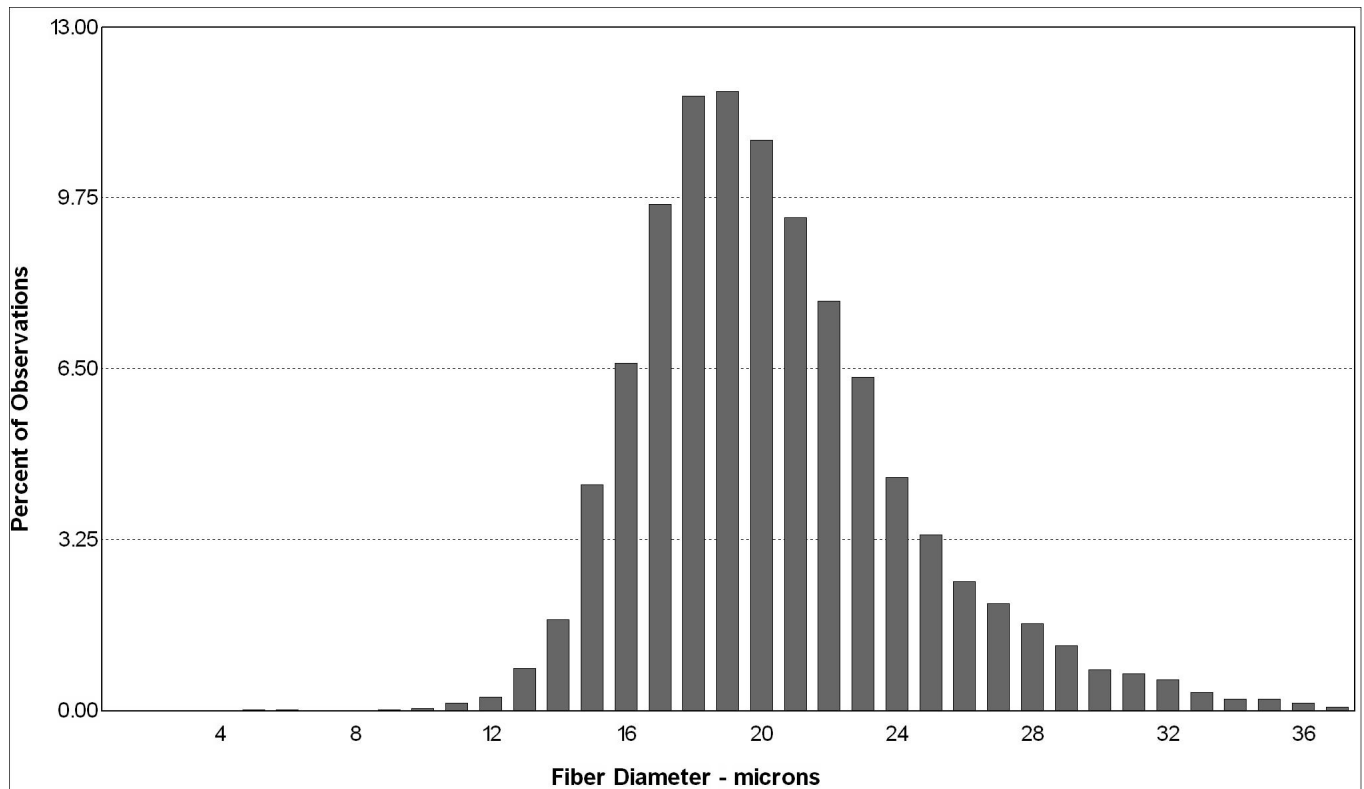

This Test Performed According to I.W.T.O Method 47