



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Brewster Alpacas/Kelly Brewster
P.O. Box 335
Bowden AB T0M 0K0 Canada

03/26/19

Test No: 973278


Animal and Sample Description

Animal Name: Halle
Breed: Alpaca(Huacaya)
Sex: Female
Color: Med Fawn

Animal ID: XXXXX
Sample Location: Side (L)
Sample Date: 05/04/18
Age: 08/23/12

Laboratory Data

Mean Fiber Diameter: 25.7 microns
Standard Deviation: 4.7 microns
Coefficient of Variation: 18.4 %
Fibers Greater Than 30 microns: 14.1 %

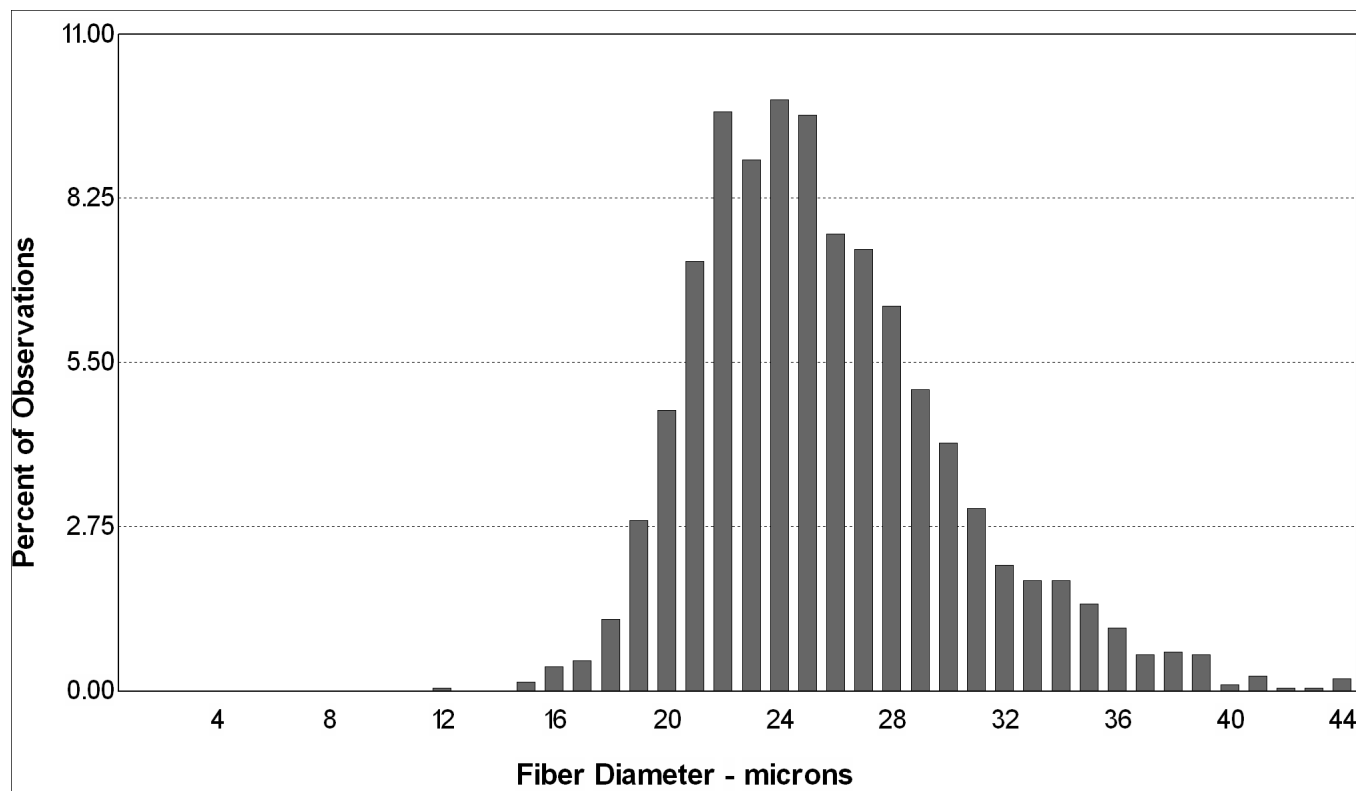

This Test Performed According to I.W.T.O Method 12