

## Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

### Sirolan Laserscan Micron Test Report

Pacesetter Alpacas/Dennis Pace  
5546 W Plymouth Church Rd  
Beloit WI 53511 USA

09/03/15

Test No: 913797


#### Animal and Sample Description

**Animal Name:** Mayhem  
**Breed:** Alpaca(Suri)  
**Sex:** Male  
**Color:** Brown

**Animal ID:** XXXXX  
**Sample Location:** Side  
**Sample Date:** 04/23/15  
**Age:** 06/16/14

#### Laboratory Data

**Mean Fiber Diameter:** 21.7 microns  
**Standard Deviation:** 4.9 microns  
**Coefficient of Variation:** 22.5 %  
**Fibers Greater Than 30 microns:** 5.1 %

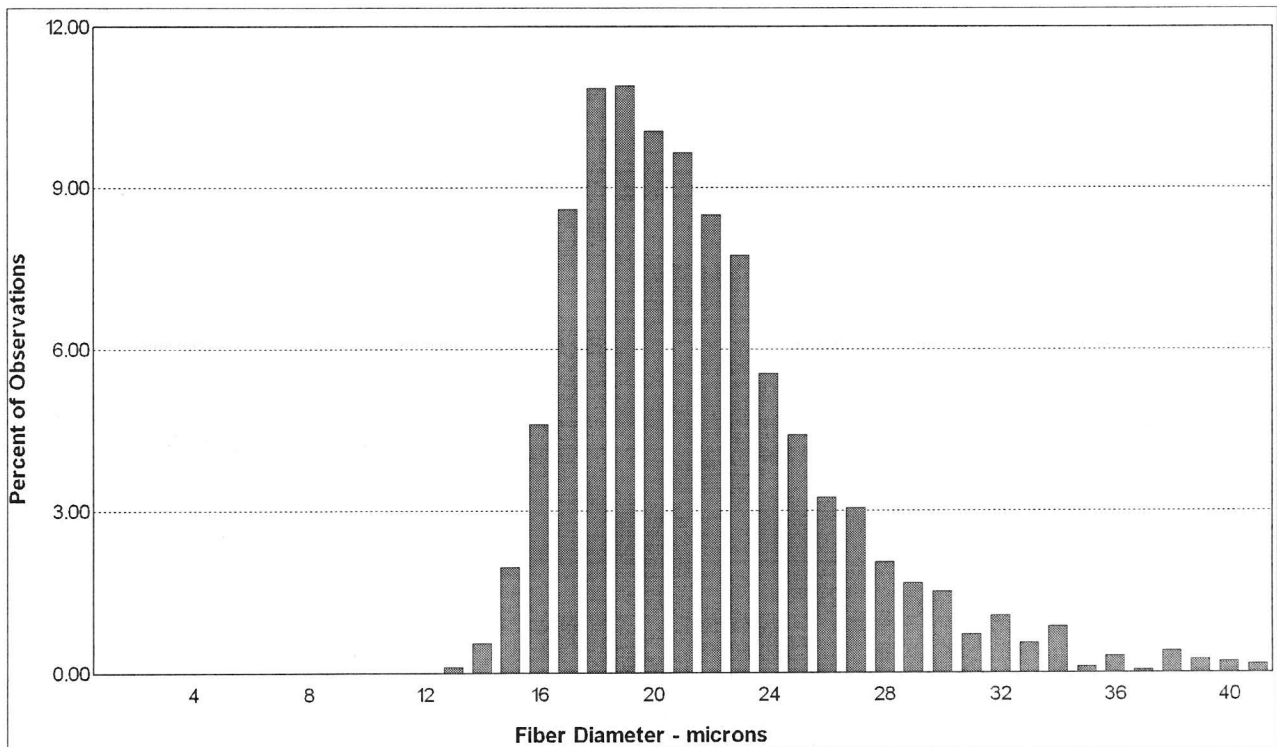

This Test Performed According to I.W.T.O Method 12