

# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Pacesetter Alpacas/Dennis Pace  
5546 W Plymouth Church Rd  
Beloit WI 53511 USA

08/13/12

Test No: 439255


### Animal and Sample Description

**Animal Name:** Kingston  
**Breed:** Alpaca(Suri)  
**Sex:** Male  
**Color:** Beige

**Animal ID:** 32203905  
**Sample Location:** Side  
**Sample Date:** 05/09/12  
**Age:** 05/18/11

### Laboratory Data

**Mean Fiber Diameter:** 17.0 microns  
**Standard Deviation:** 2.7 microns  
**Coefficient of Variation:** 15.8 %  
**Fibers Greater Than 30 microns:** 0.5 %

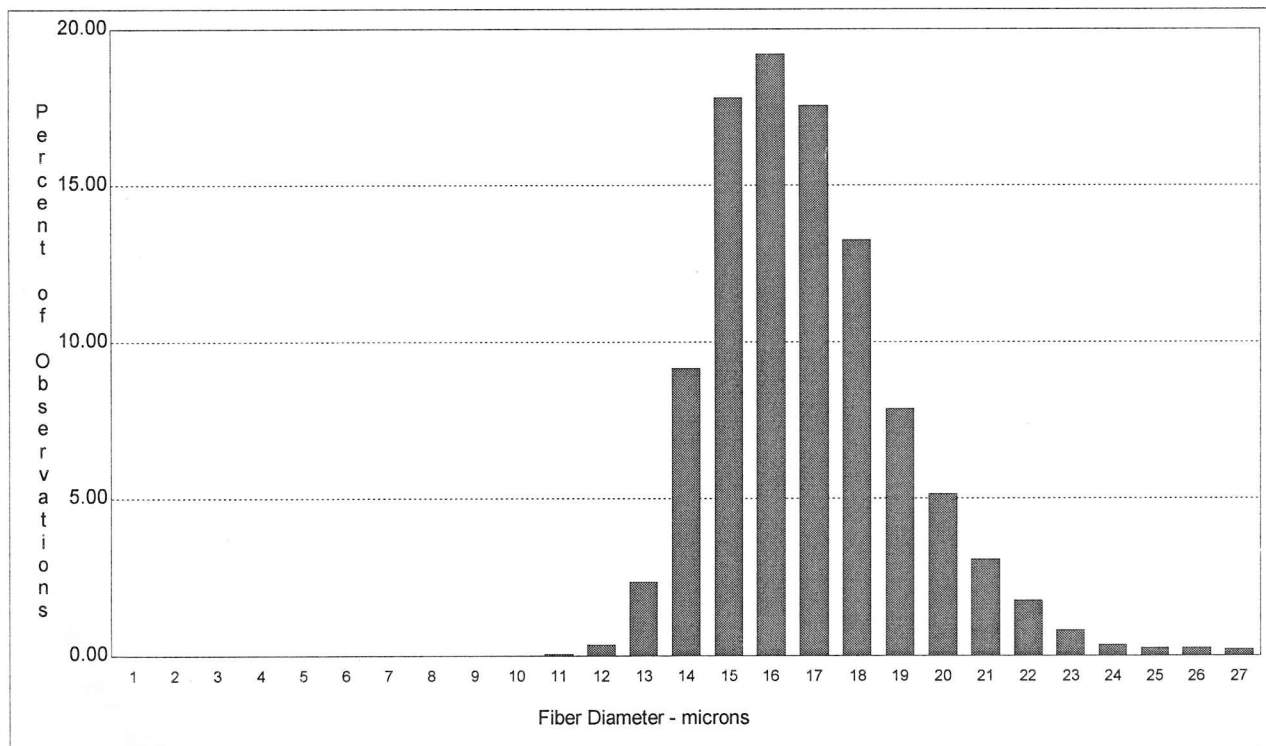

This Test Performed According to I.W.T.O Method 12