

# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Skyline Alpacas/Mary Jaffe  
11100 NW Saltzman Rd  
Portland OR 97229 USA

08/05/13

Test No: 464107


### Animal and Sample Description

**Animal Name:** Gunsmoke  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** Lt Silver Grey

**Animal ID:** 31974127  
**Sample Location:** Side  
**Sample Date:** 05/02/13  
**Age:** 06/02/11

### Laboratory Data

**Mean Fiber Diameter:** 24.5 microns  
**Standard Deviation:** 4.0 microns  
**Coefficient of Variation:** 16.3 %  
**Fibers Greater Than 30 microns:** 6.6 %

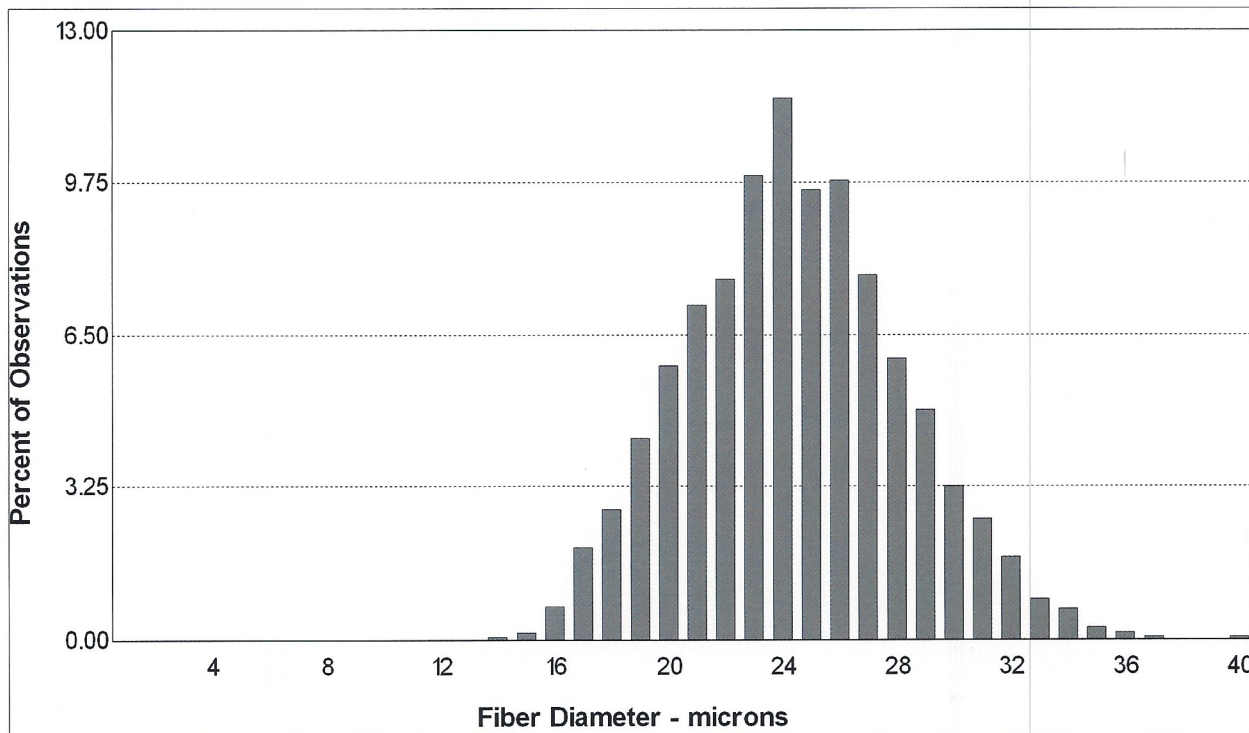

This Test Performed According to I.W.T.O Method 12