

# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

R & R Ranch/Richard & Robin Vasquez  
325B Denio Avenue  
Gilroy CA 95020-9203 USA

07/19/10

Test No: 384128


### Animal and Sample Description

**Animal Name:** Shazaam  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** Beige

**Animal ID:** 1019957  
**Sample Location:** Side  
**Sample Date:** 06/03/10  
**Age:** 08/24/03

### Laboratory Data

**Mean Fiber Diameter:** 29.3 microns  
**Standard Deviation:** 5.8 microns  
**Coefficient of Variation:** 19.8 %  
**Fibers Greater Than 30 microns:** 36.3 %

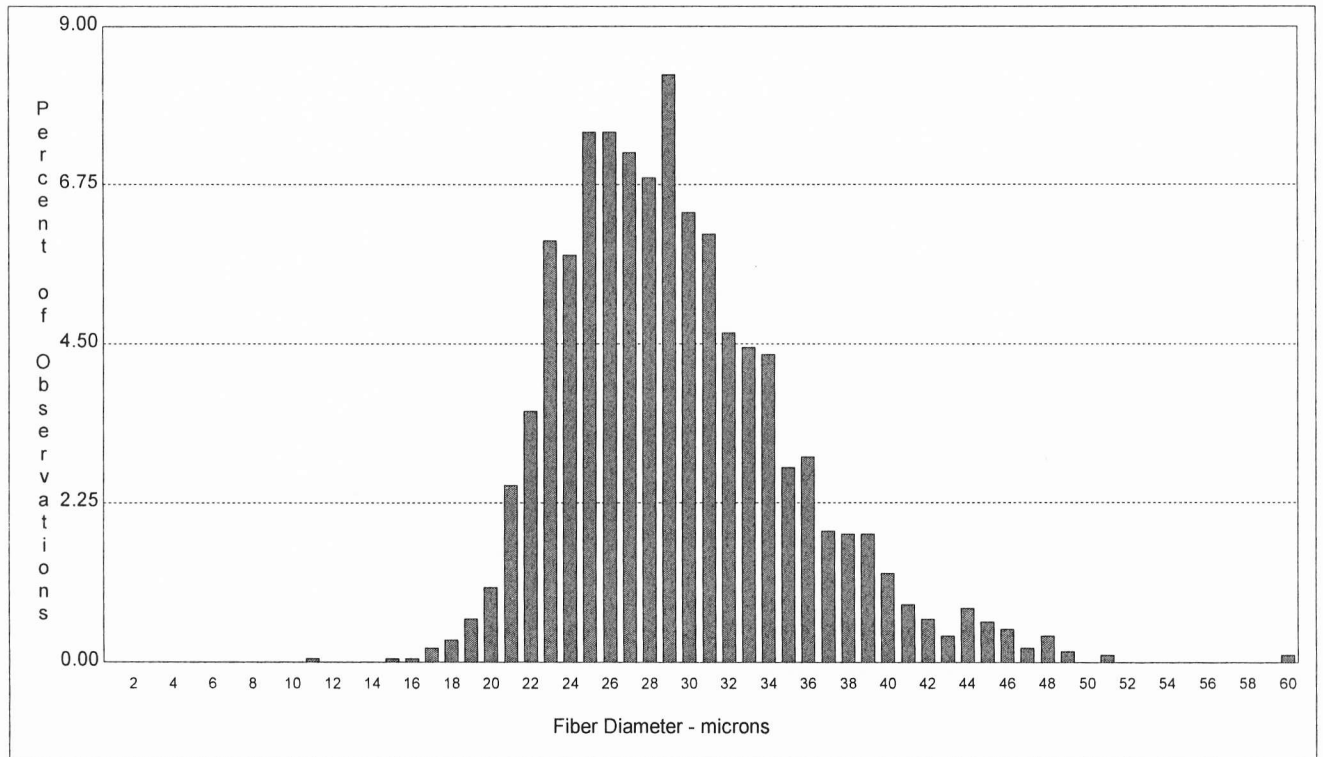

This Test Performed According to I.W.T.O Method 12