



**Yocom-McColl Testing Laboratories, Inc.**  
540 West Elk Place • Denver, Colorado 80216-1823 USA  
PHONE (303) 294-0582 • FAX (303) 295-6944  
EMAIL: ymccoll@ymccoll.com

**Sirolan Laserscan  
Micron Test Report**

The Wood Farm/Libby Stover  
14 Wood Road  
Franklin PA 16323 U.S.A

06/26/14

Test No: 482614


**Animal and Sample Description**

**Animal Name:** TWF Peruvian Carmen  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Med Fawn

**Animal ID:** 32653793  
**Sample Location:** Mid Side  
**Sample Date:** 05/23/14  
**Age:** 09/22/13

**Laboratory Data**

**Mean Fiber Diameter:** 13.9 microns  
**Standard Deviation:** 3.2 microns  
**Coefficient of Variation:** 23.1 %  
**Fibers Greater Than 30 microns:** 0.6 %

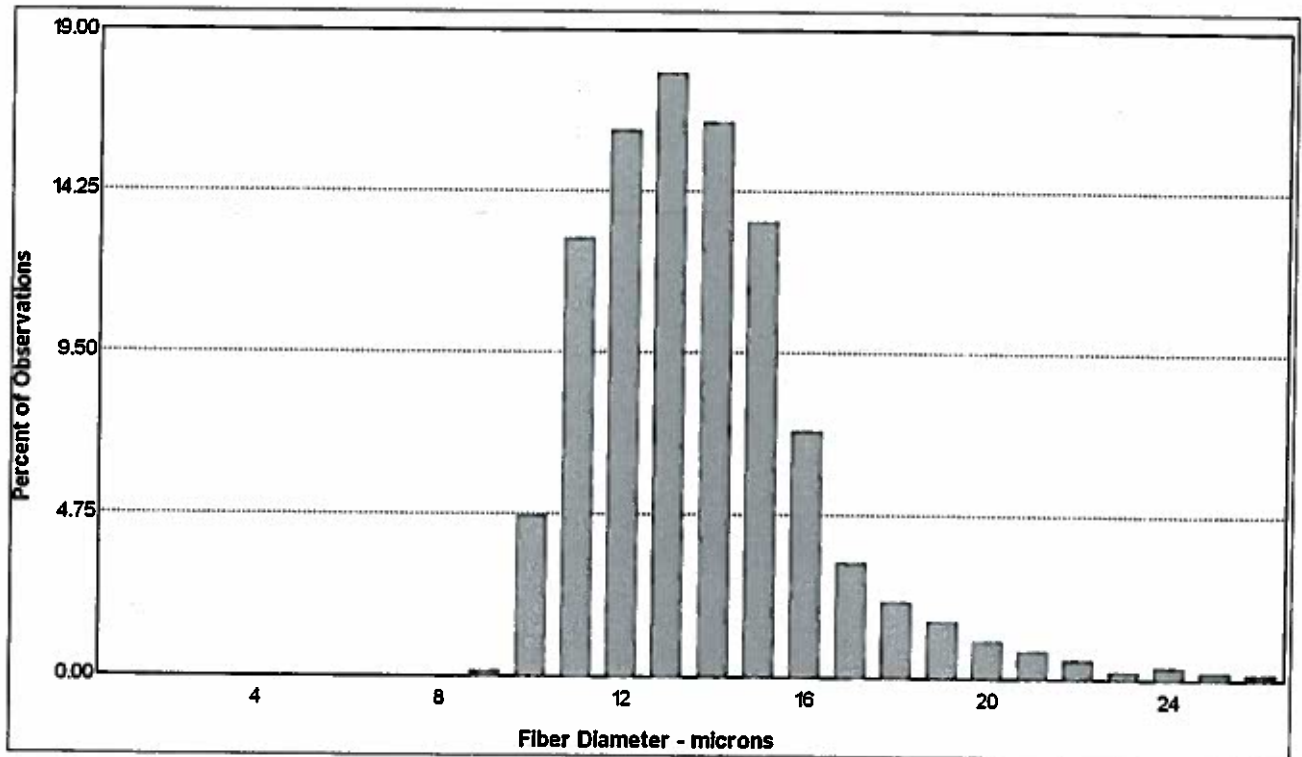

**This Test Performed According to I.W.T.O Method 12**