



Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

**Sirojan Laserscan
Micron Test Report**

The Wood Farm/Libby Stover
14 Wood Road
Franklin PA 16323 U.S.A

06/26/14

Test No: 482609


Animal and Sample Description

Animal Name: TWF Peruvian The Levitator
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: 32484519
Sample Location: Mid Side
Sample Date: 05/23/14
Age: 08/01/12

Laboratory Data

Mean Fiber Diameter: 17.9 microns
Standard Deviation: 4.3 microns
Coefficient of Variation: 24.1 %
Fibers Greater Than 30 microns: 1.4 %

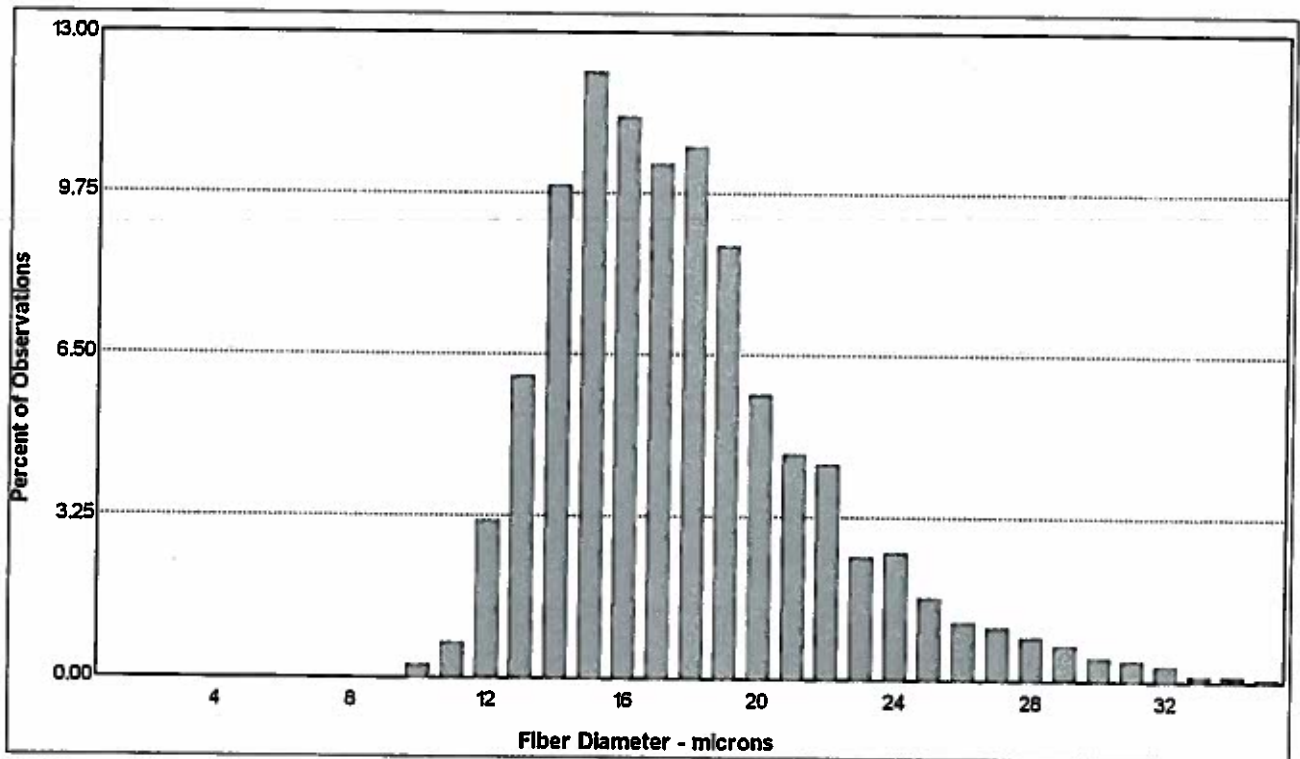

This Test Performed According to I.W.T.O Method 12