

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

West Penn Alpacas/Mike & Debbie Vigus
1843 E. Finley Dr
Claysville PA 15323 USA

Date: 06/01/16

Test No: 921408


Animal and Sample Description

Animal Name: WP Elite Emeera (2015)
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 35242291
Sample Location: Side (L)
Sample Date: 04/28/15
Age: 12/03/14

Laboratory Data

Mean Fiber Diameter:	17.5 microns	Fibers Greater Than 30 microns:	0.8 %
Standard Deviation:	4.2 microns	Comfort Factor:	99.2 %
Coefficient of Variation:	24.1 %	Mean Curvature:	42.2 deg/mm
Spin Fineness:	17.5 microns	SD Curvature:	22.6 deg/mm

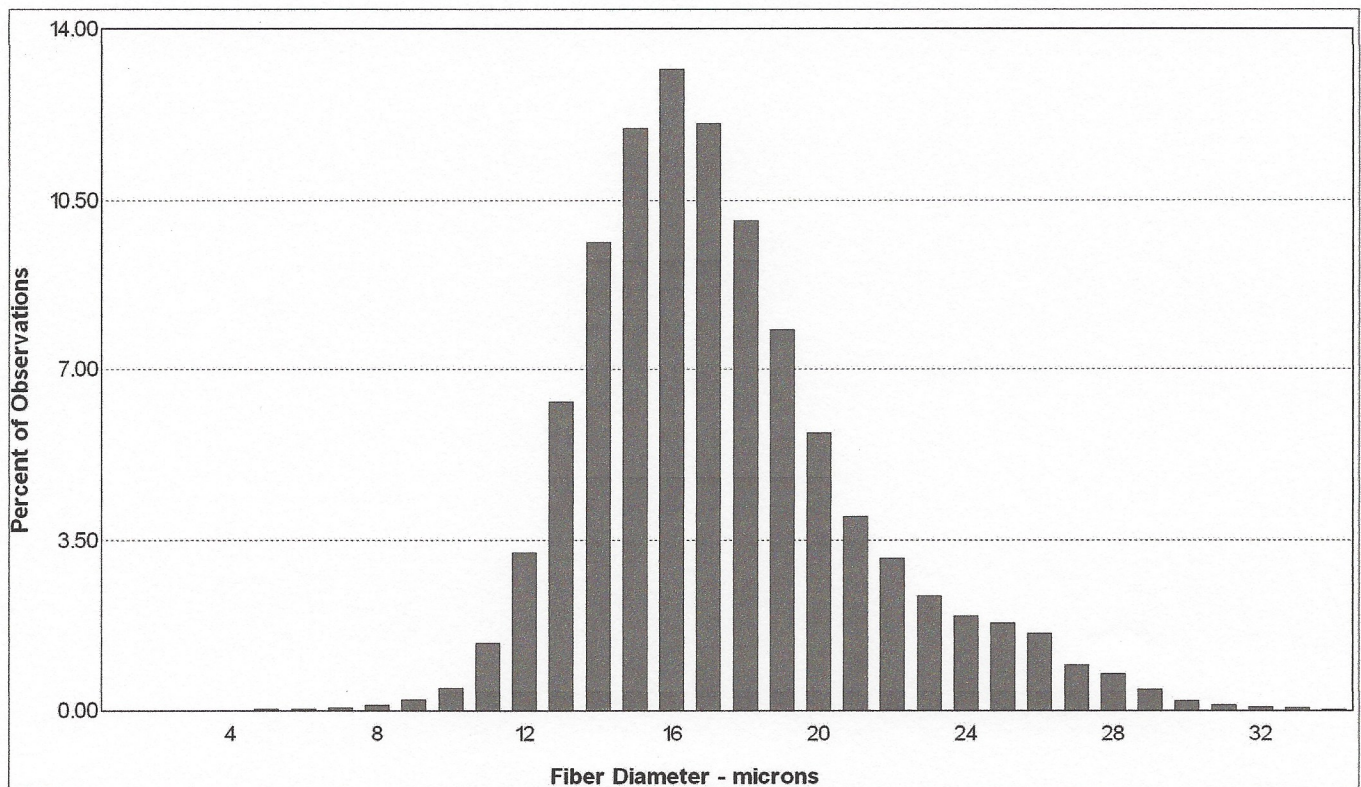

This Test Performed According to I.W.T.O Method 47