



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Glengary Farm Alpacas/Patrick Cassese  
2704 Slessman Drive  
Plymouth OH 44865 USA

**Date:** 07/03/18

**Test No:** 962521


### Animal and Sample Description

**Animal Name:** GGF Midnight Aphrodite  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Black

**Animal ID:** 35453802  
**Sample Location:** Side  
**Sample Date:** 04/28/18  
**Age:** 08/04/17

### Laboratory Data

<b>Mean Fiber Diameter:</b>	18.9 microns	<b>Fibers Greater Than 30 microns:</b>	3.0 %
<b>Standard Deviation:</b>	4.7 microns	<b>Comfort Factor:</b>	97.0 %
<b>Coefficient of Variation:</b>	24.7 %	<b>Mean Curvature:</b>	32.1 deg/mm
<b>Spin Fineness:</b>	19.0 microns	<b>SD Curvature:</b>	20.6 deg/mm

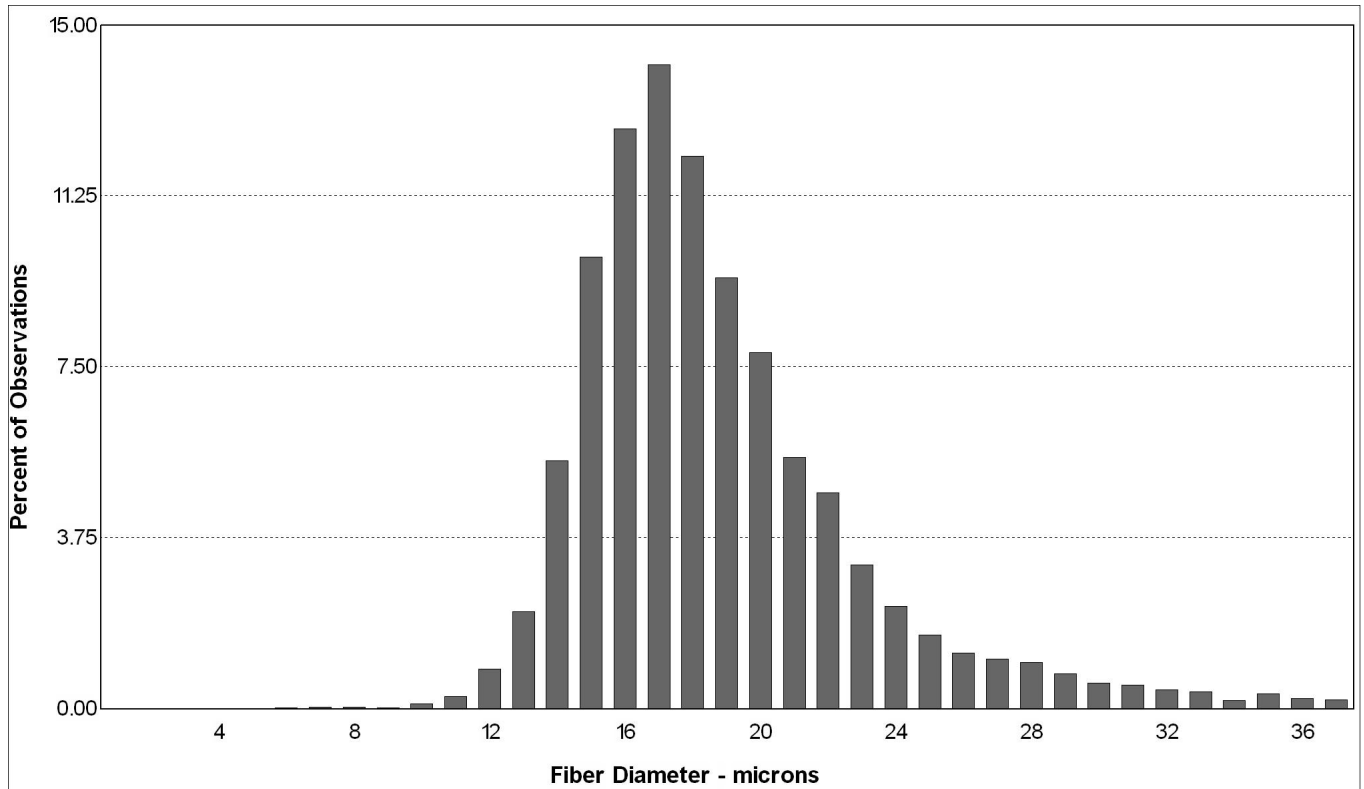

This Test Performed According to I.W.T.O Method 47