



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Cabin View Alpacas/Christine & David Houseworth  
9435 Congress St Ext  
Trumansburg NY 14886 USA

06/30/16

Test No: 925614


### Animal and Sample Description

**Animal Name:** CVAF Daisy Mae  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Lt Fawn

**Animal ID:** 32636673  
**Sample Location:** Mid Side  
**Sample Date:** 05/21/16  
**Age:** 07/27/15

### Laboratory Data

**Mean Fiber Diameter:** 18.9 microns  
**Standard Deviation:** 3.4 microns  
**Coefficient of Variation:** 17.8 %  
**Fibers Greater Than 30 microns:** 0.7 %

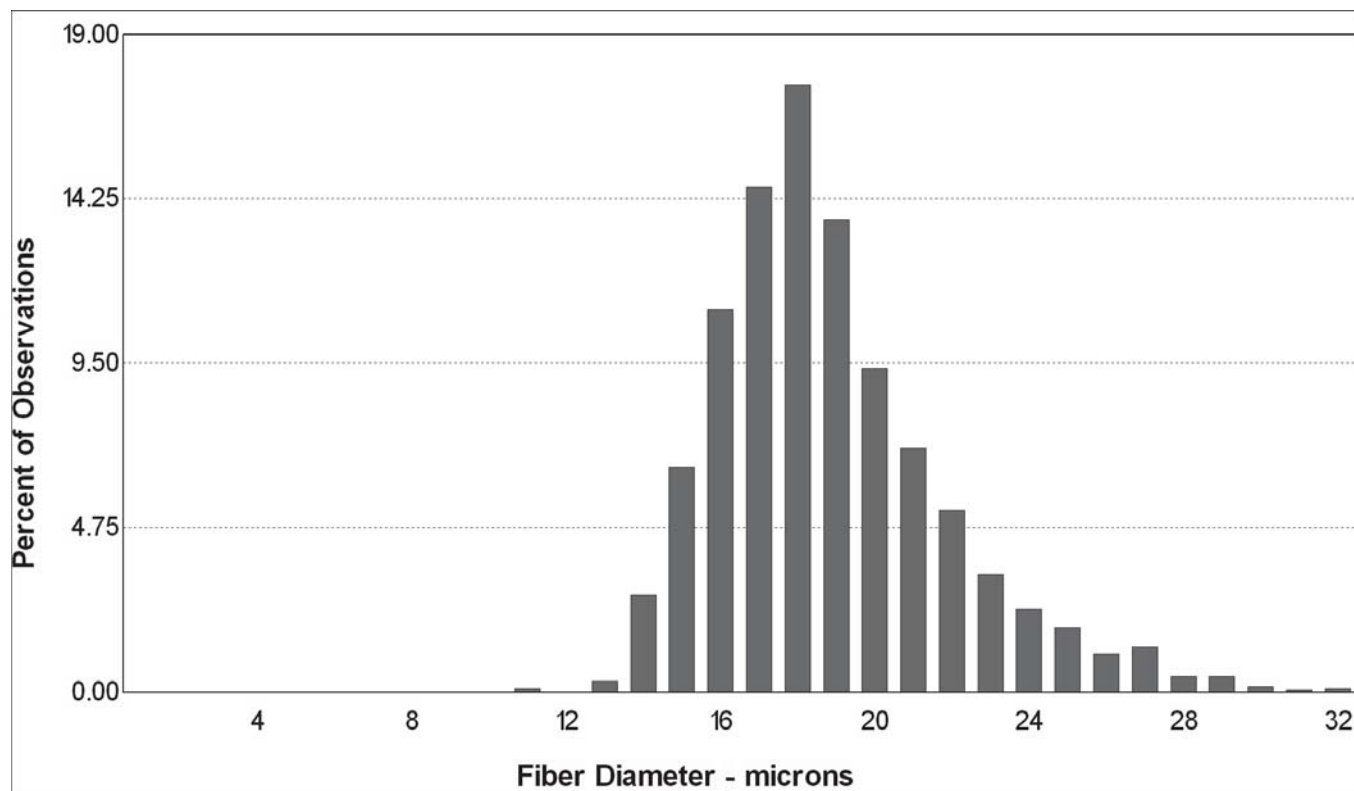

This Test Performed According to I.W.T.O Method 12