



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Cabin View Alpacas/Christine & David Houseworth  
9435 Congress St Ext  
Trumansburg NY 14886 USA

06/27/18

Test No: 962243


### Animal and Sample Description

**Animal Name:** VAF Peruvian Texas May  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** XXXXX

**Animal ID:** 31555494  
**Sample Location:** Side  
**Sample Date:** 05/14/18  
**Age:** 05/05/09

### Laboratory Data

<b>Mean Fiber Diameter:</b>	22.1 microns	<b>Spin Fineness:</b>	21.8 microns
<b>Standard Deviation:</b>	5.0 microns	<b>Mean Curvature (deg/mm):</b>	42.5
<b>Coefficient of Variation:</b>	22.4 %	<b>SD Curvature (deg/mm):</b>	26.9
<b>Fibers Greater Than 30 microns:</b>	6.4 %	<b>Comfort Factor:</b>	93.6 %

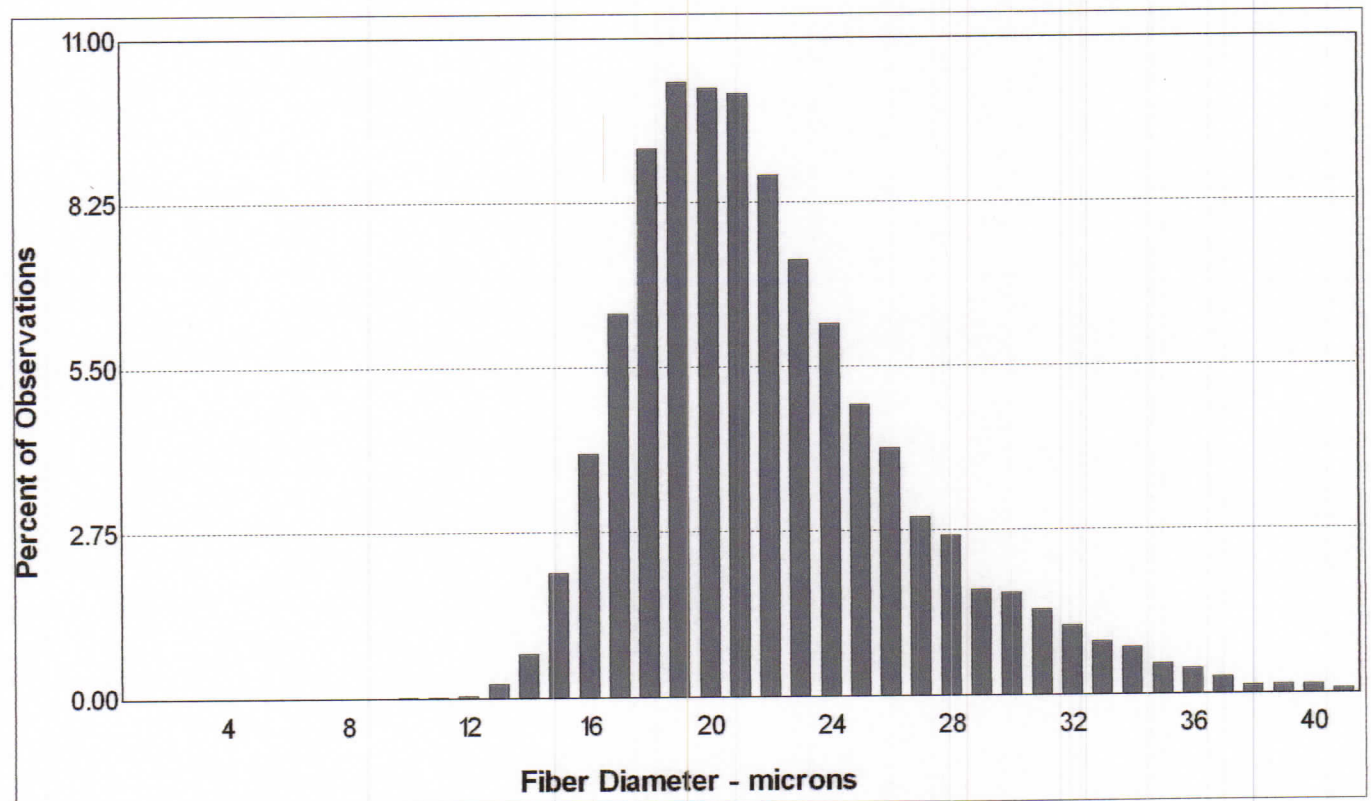

This Test Performed According to I.W.T.O Method 47