



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Cinco C's Alpacas/Carol Howard  
198 Sartwell Creek Road  
Port Allegany PA 16743

08/02/12

Test No: 437107


### Animal and Sample Description

**Animal Name:** 5C's Cascade of Sparks  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** XXXXX

**Animal ID:** 31754859  
**Sample Location:** Side  
**Sample Date:** 05/20/12  
**Age:** 08/30/09

### Laboratory Data

**Mean Fiber Diameter:** 18.4 microns  
**Standard Deviation:** 4.2 microns  
**Coefficient of Variation:** 22.9 %  
**Fibers Greater Than 30 microns:** 2.0 %

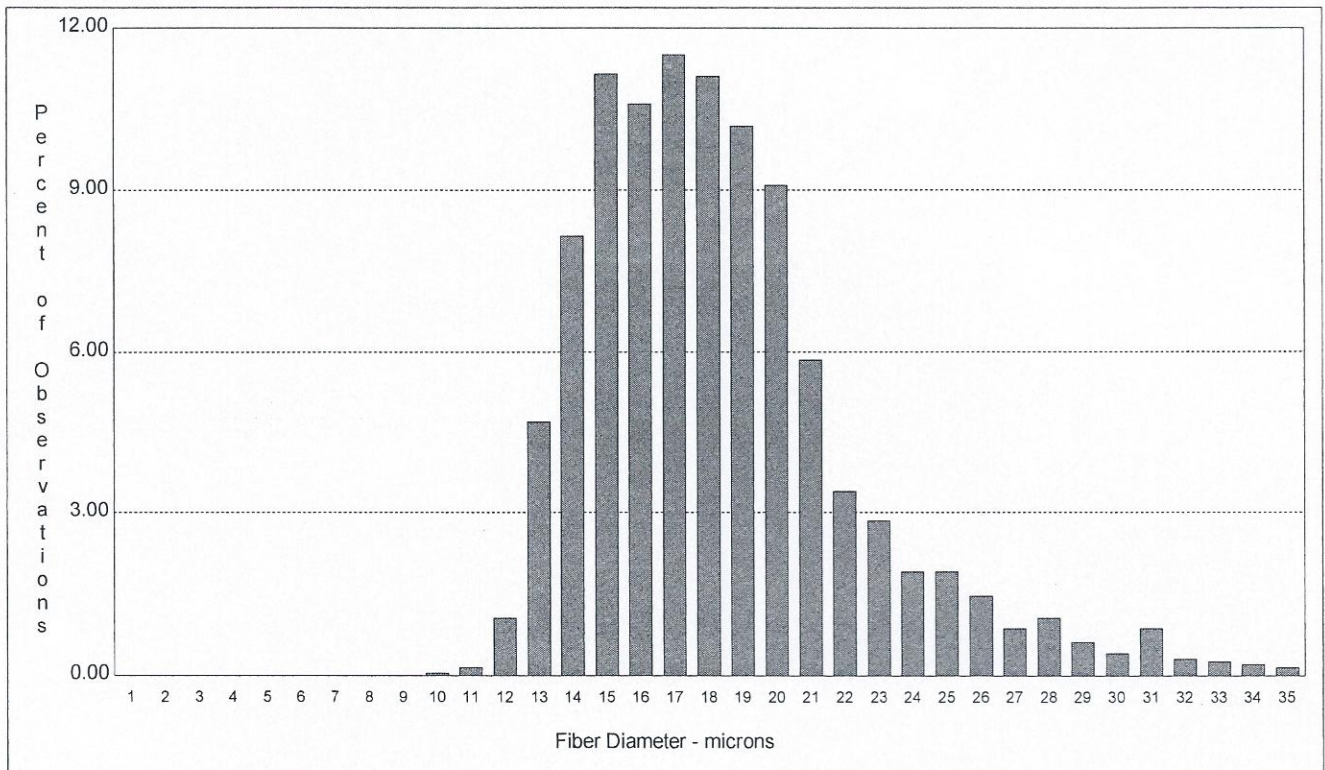

This Test Performed According to I.W.T.O Method 12