

# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Rogue Suri Alpacas/Jason & Beverly Brehm  
1075 Washburn Lane  
Medford OR 97501 USA

Date: 02/17/16

Test No: 918828


### Animal and Sample Description

**Animal Name:** RGSA Versace  
**Breed:** Alpaca(Suri)  
**Sex:** Female  
**Color:** Lt Fawn

**Animal ID:** 35267171  
**Sample Location:** Side (R)  
**Sample Date:** 02/11/16  
**Age:** 07/23/15

### Laboratory Data

<b>Mean Fiber Diameter:</b>	18.5 microns	<b>Fibers Greater Than 30 microns:</b>	0.9 %
<b>Standard Deviation:</b>	3.9 microns	<b>Comfort Factor:</b>	99.1 %
<b>Coefficient of Variation:</b>	20.8 %	<b>Mean Curvature:</b>	13.4 deg/mm
<b>Spin Fineness:</b>	18.0 microns	<b>SD Curvature:</b>	18.5 deg/mm

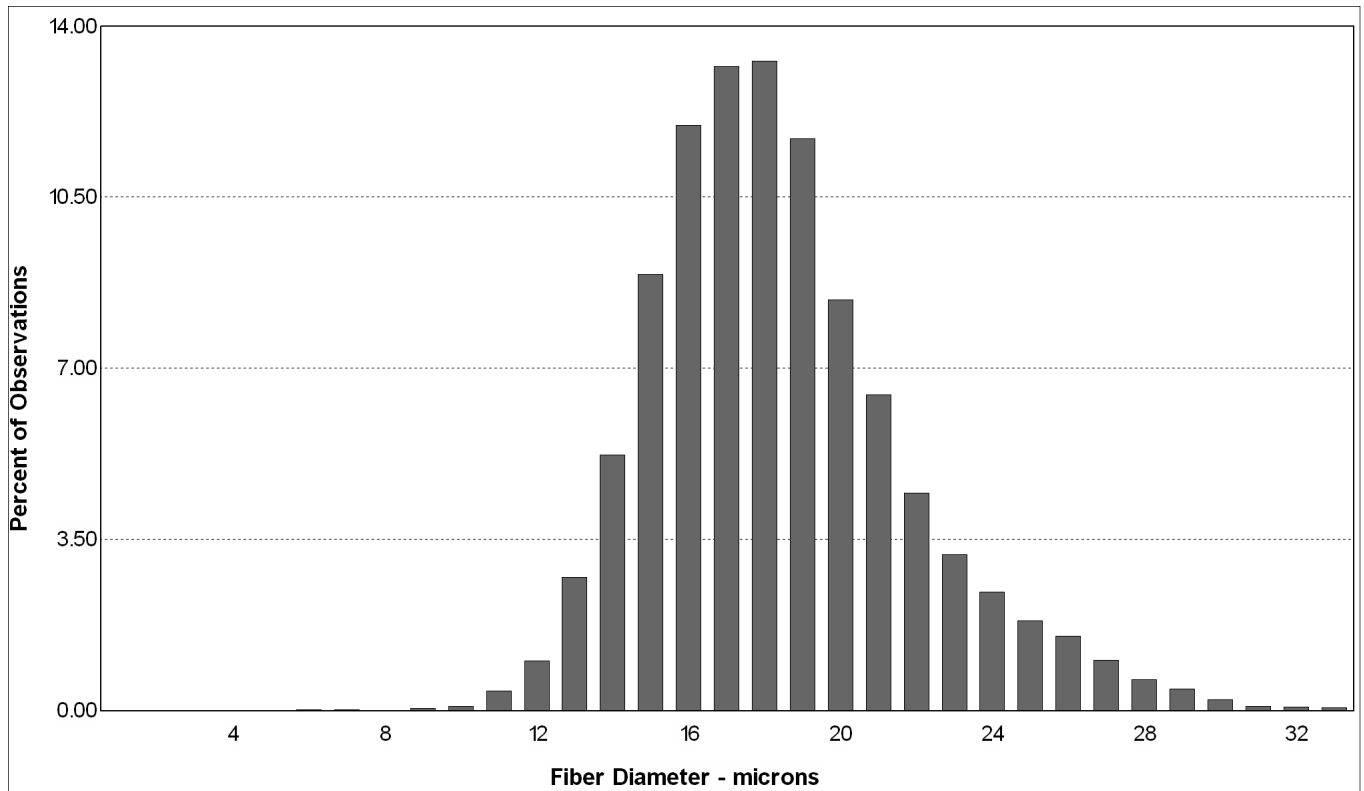

This Test Performed According to I.W.T.O Method 47