



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

The Wood Farm/Libby Stover
14 Wood Road
Franklin PA 16323 USA

11/14/17

Test No: 955306


Animal and Sample Description

Animal Name: TWF Peruvian Cerveza
Breed: Alpaca(Huacaya)
Sex: Male
Color: Beige

Animal ID: 35128458
Sample Location: Side (L)
Sample Date: 05/22/17
Age: 08/18/16

Laboratory Data

Mean Fiber Diameter: 14.6 microns
Standard Deviation: 2.8 microns
Coefficient of Variation: 18.9 %
Fibers Greater Than 30 microns: 0.1 %

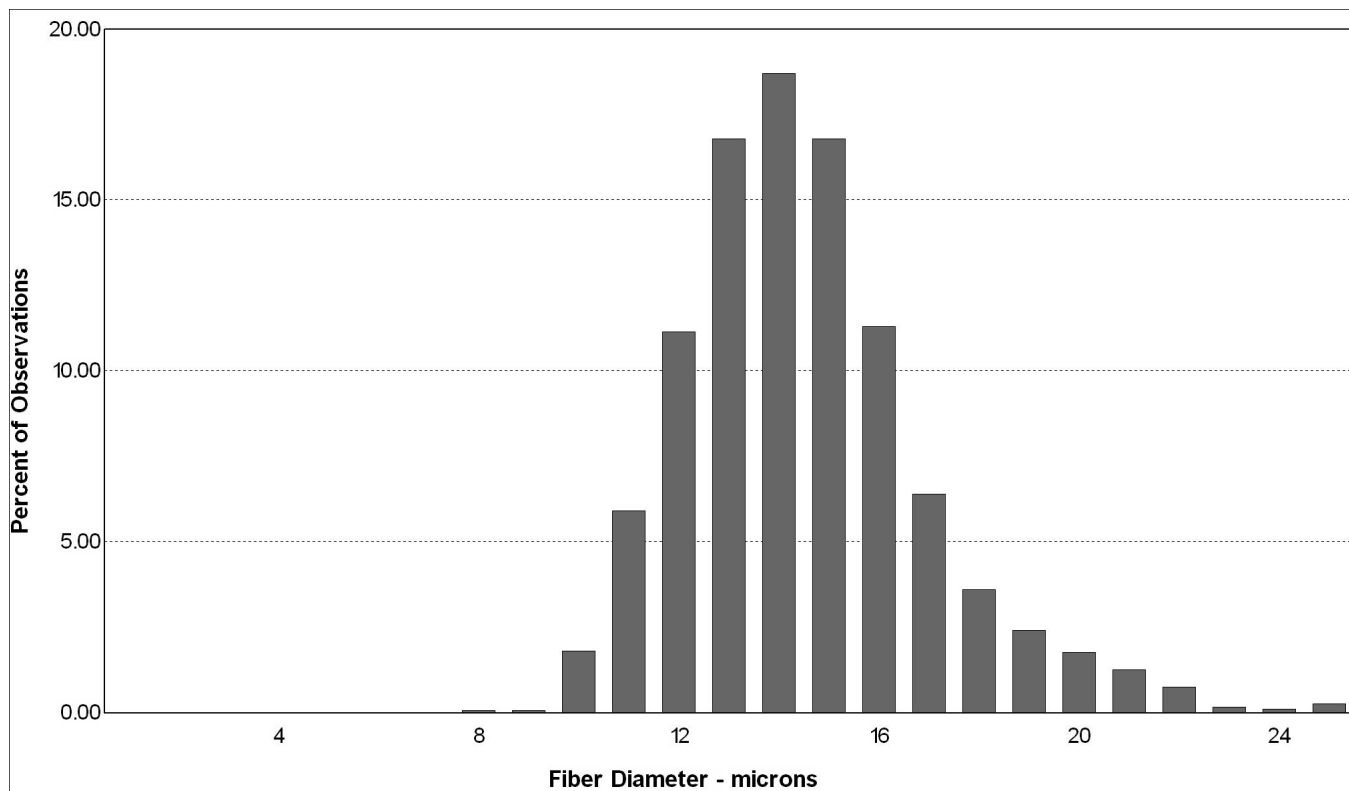

This Test Performed According to I.W.T.O Method 12