



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

OakHill Alpacas, LLC/Joyce Calderwood
7226 First Avenue
Mays Landing NJ 08330 USA

08/05/14

Test No: 488902


Animal and Sample Description

Animal Name: NJOakhill's Nakita
Breed: Alpaca(Huacaya)
Sex: Female
Color: True Black

Animal ID: XXXXX
Sample Location: Side
Sample Date: 05/08/14
Age: 06/17/13

Laboratory Data

Mean Fiber Diameter: 21.4 microns
Standard Deviation: 4.6 microns
Coefficient of Variation: 21.5 %
Fibers Greater Than 30 microns: 4.9 %

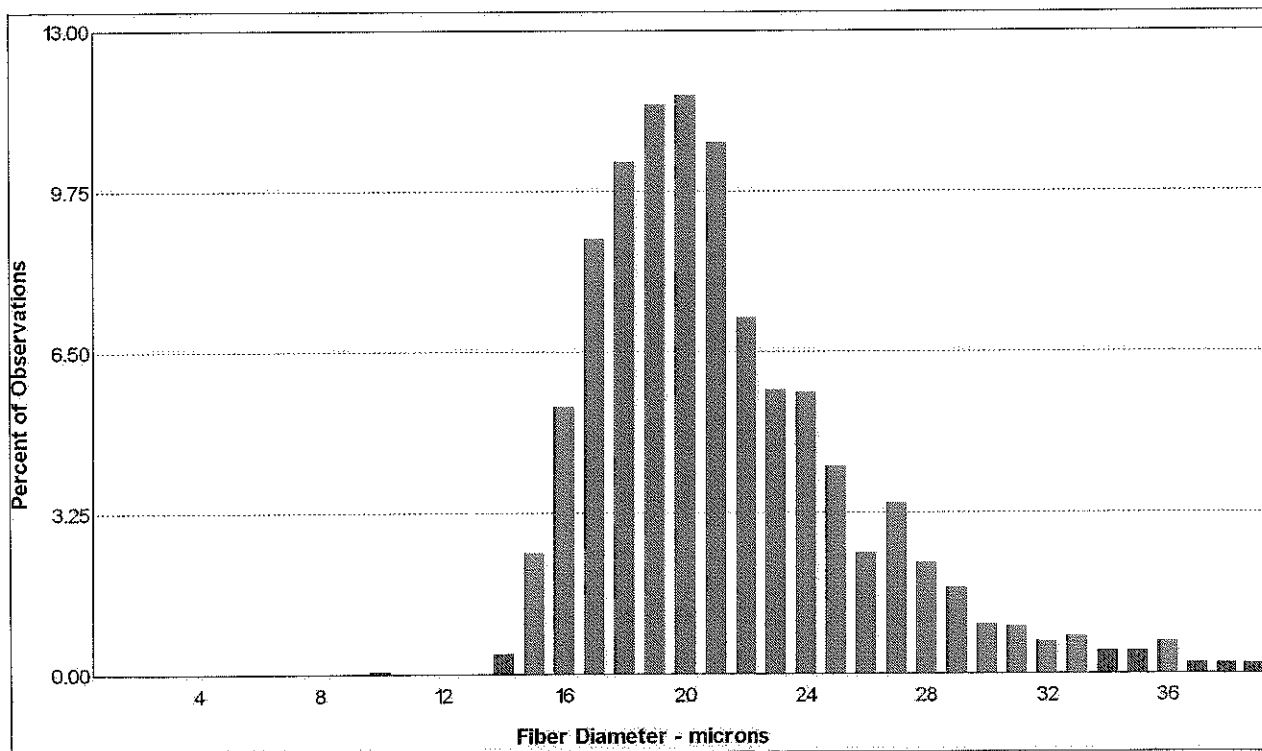

This Test Performed According to I.W.T.O Method 12