



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Pleasant Journey Alpacas/Susan Kacsh  
4128 County Road 129  
Hesperus CO 81326 USA

**Date:** 07/27/16

**Test No:** 927849


### Animal and Sample Description

**Animal Name:** Annual's Chrome Finish  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** Lt Silver Grey

**Animal ID:** 35066309  
**Sample Location:** Side  
**Sample Date:** 05/08/16  
**Age:** 07/10/14

### Laboratory Data

<b>Mean Fiber Diameter:</b>	17.6 microns	<b>Fibers Greater Than 30 microns:</b>	0.6 %
<b>Standard Deviation:</b>	3.5 microns	<b>Comfort Factor:</b>	99.4 %
<b>Coefficient of Variation:</b>	20.1 %	<b>Mean Curvature:</b>	49.7 deg/mm
<b>Spin Fineness:</b>	17.0 microns	<b>SD Curvature:</b>	26.2 deg/mm

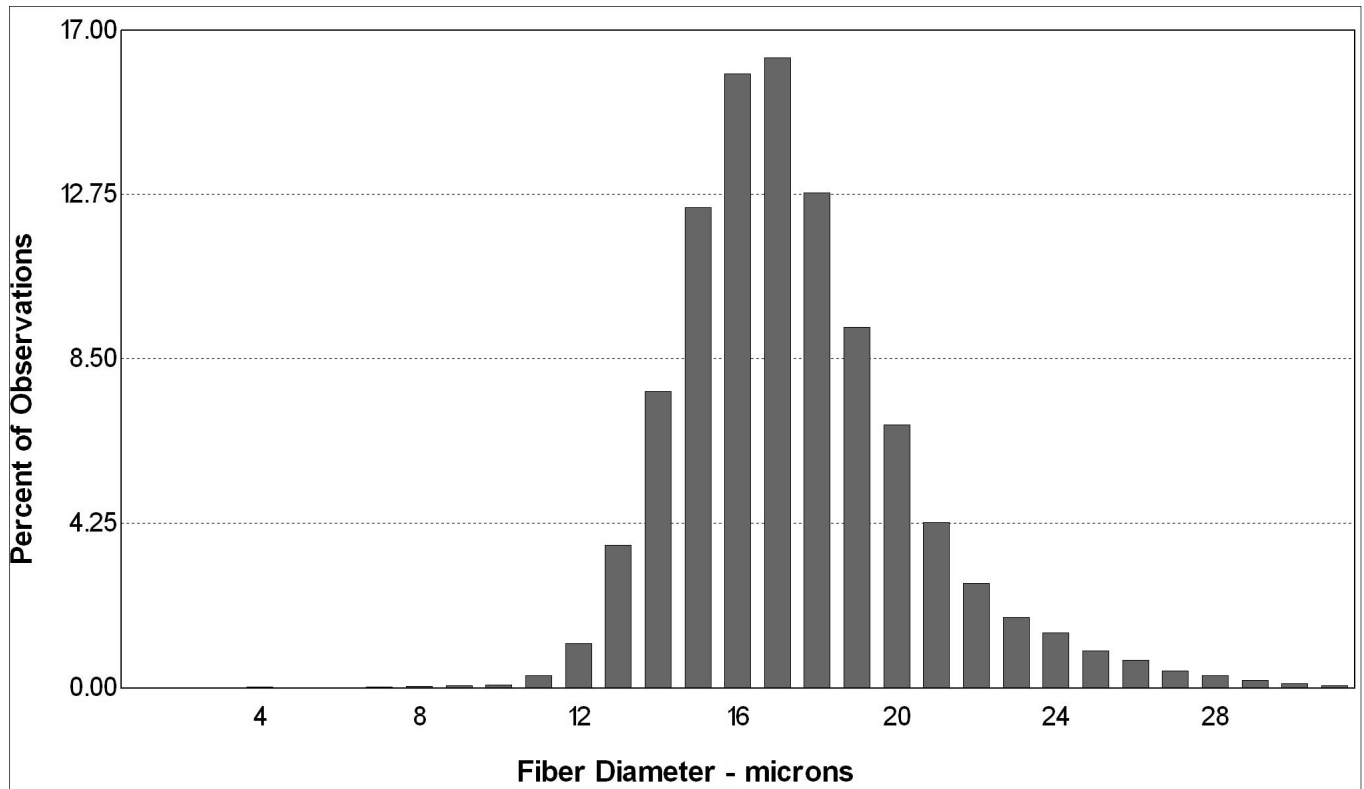

This Test Performed According to I.W.T.O Method 47