



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Pleasant Journey Alpacas/Susan Kacsh  
4128 County Road 129  
Hesperus CO 81326 USA

Date: 01/19/15

Test No: 496540


### Animal and Sample Description

**Animal Name:** PJA Caramel Sundae  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Lt Fawn

**Animal ID:** 32657678  
**Sample Location:** Side  
**Sample Date:** 05/24/14  
**Age:** 09/08/13

### Laboratory Data

<b>Mean Fiber Diameter:</b>	19.3 microns	<b>Fibers Greater Than 30 microns:</b>	2.2 %
<b>Standard Deviation:</b>	4.4 microns	<b>Comfort Factor:</b>	97.8 %
<b>Coefficient of Variation:</b>	23.0 %	<b>Mean Curvature:</b>	38.2 deg/mm
<b>Spin Fineness:</b>	19.1 microns	<b>SD Curvature:</b>	23.3 deg/mm

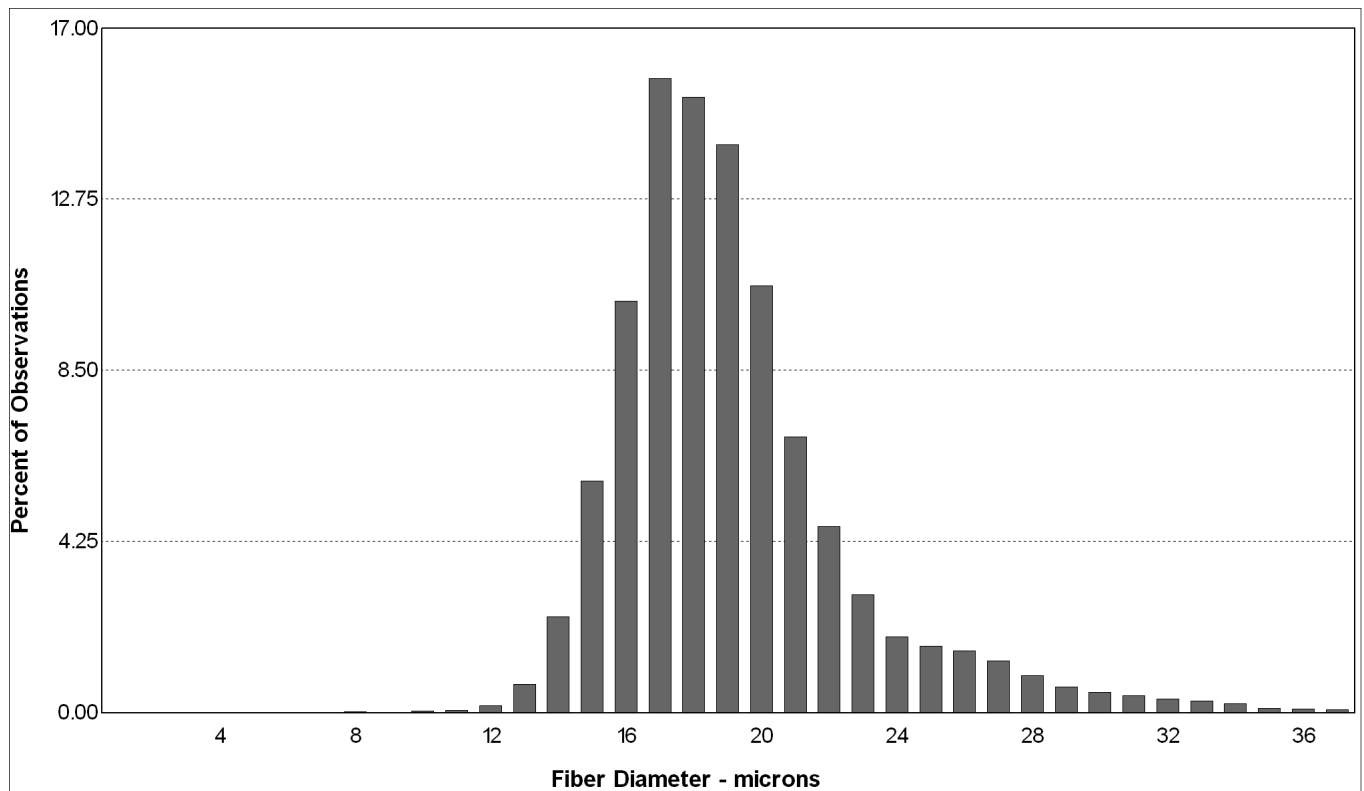

This Test Performed According to I.W.T.O Method 47