

# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Alpacas at Windy Hill/Cindy Harris  
8575 Waters Rd  
Moorpark CA 93021 USA

**Date:** 10/03/12  
**Shear ID:** 27437  
**Test No:** 439464


### Animal and Sample Description

**Animal Name:** Pucara Hannah  
**ARI #:** 1340044  
**Breed:** Alpaca(Suri)  
**Sex:** Female  
**Color:** White

**Date of Birth (Age):** 11/05/04  
**Sample Location:** Side  
**Sample Date:** 04/22/11  
**Previous Shear Date:** 04/02/10  
**Total Fleece Wt (lbs):** 4.20

### Laboratory Data

<b>Mean Fiber Diameter:</b>	29.4 microns	<b>Mean Staple Length:</b>	124.4 mm
<b>Standard Deviation:</b>	6.2 microns	<b>Length Standard Deviation:</b>	7.1 mm
<b>Coefficient of Variation:</b>	21.0 %	<b>Length Coefficient of Variation:</b>	5.7 %
<b>Spin Fineness:</b>	28.7 microns	<b>Mean Curvature:</b>	9.3 deg/mm
<b>Fibers Greater Than 30 microns:</b>	32.5 %	<b>SD Curvature:</b>	11.6 deg/mm
<b>Comfort Factor:</b>	67.5 %	<b>Medullated Fibers:</b>	22.5 %

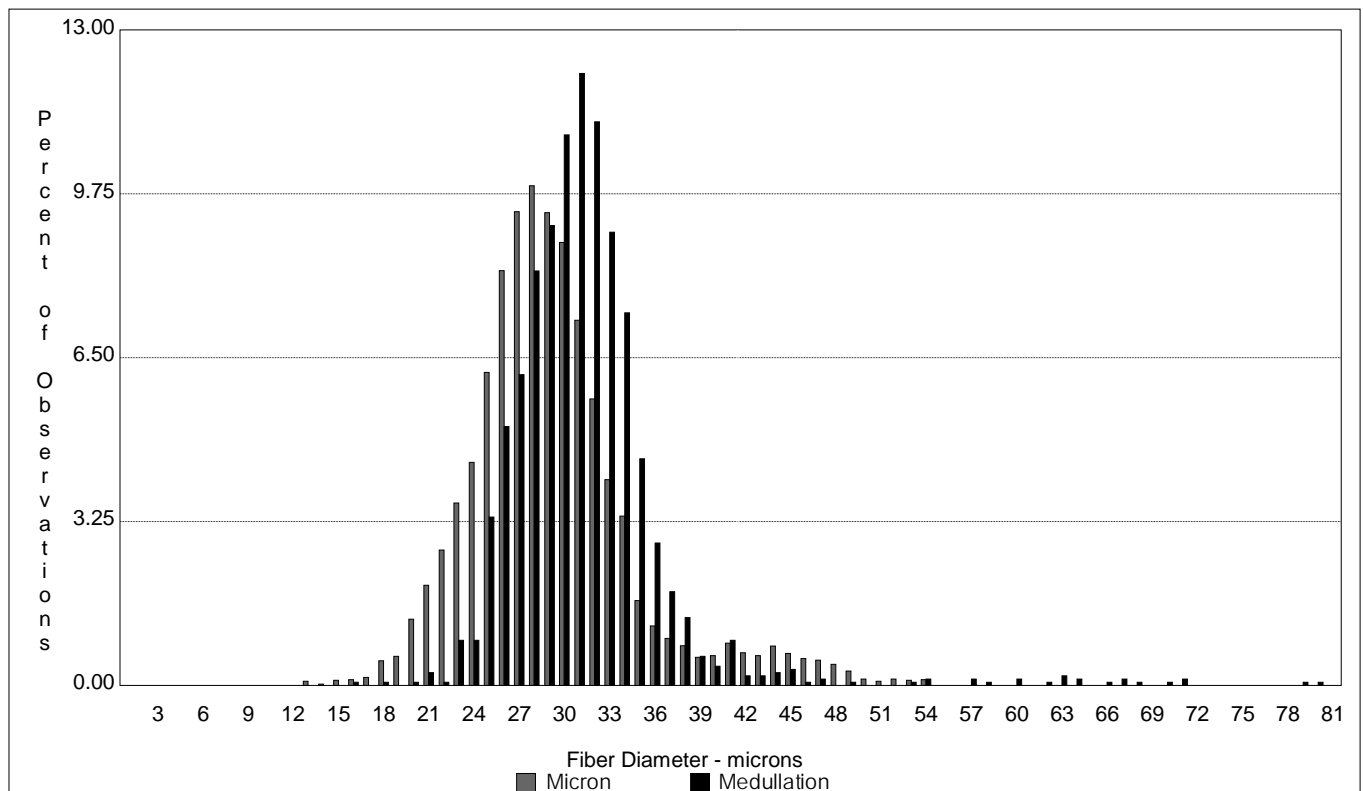

This Test Performed According to I.W.T.O Method 47