



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Pleasant Prairie Suris/Verna Carpenter
4101 N Ashton Road
Otis Orchard WA 99027 USA

Date: 07/18/16

Test No: 928213


Animal and Sample Description

Animal Name: Arya of PPS
Breed: Alpaca(Suri)
Sex: Female
Color: Lt Fawn

Animal ID: 35303701
Sample Location: Side
Sample Date: 06/04/16
Age: 06/05/15

Laboratory Data

Mean Fiber Diameter:	17.0 microns	Fibers Greater Than 30 microns:	1.2 %
Standard Deviation:	4.6 microns	Comfort Factor:	98.8 %
Coefficient of Variation:	27.0 %	Mean Curvature:	15.8 deg/mm
Spin Fineness:	17.5 microns	SD Curvature:	23.1 deg/mm

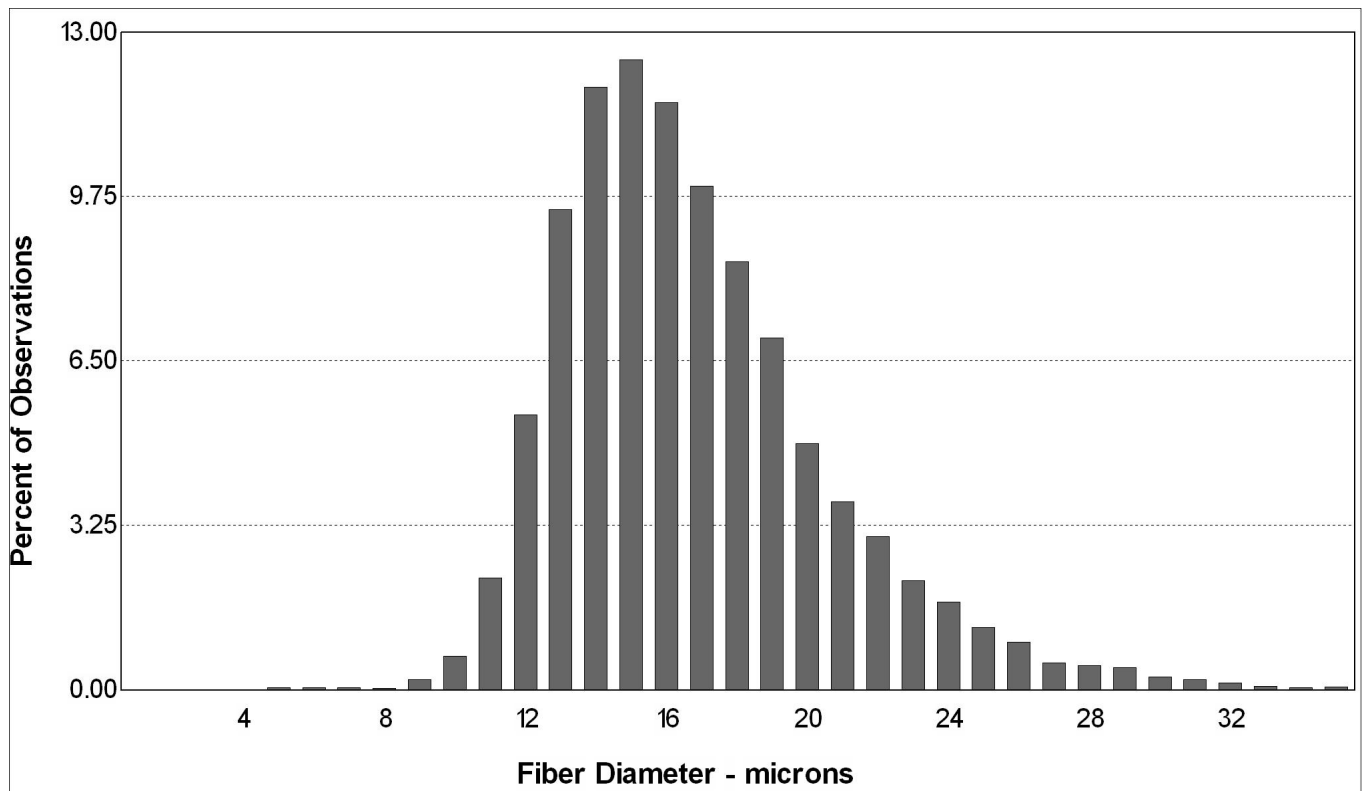

This Test Performed According to I.W.T.O Method 47