

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Likada Farm/Larry Johnson
500 Park Blvd, Ste 800
Itasca IL 60143-3169 U.S.A.

05/14/09

Test No: 348295

Animal and Sample Description


Animal Name: Margo's 2008 Cria
Breed: Alpaca(Huacaya)
Sex: XXXXX
Color: XXXXX

Macarita

Animal ID: XXXXX
Sample Location: Side
Sample Date: XX/XX/XX
Age: XXXXX

Laboratory Data

Mean Fiber Diameter: 17.0 microns
Standard Deviation: 4.5 microns
Coefficient of Variation: 26.4 %
Fibers Greater Than 30 microns: 2.1 %

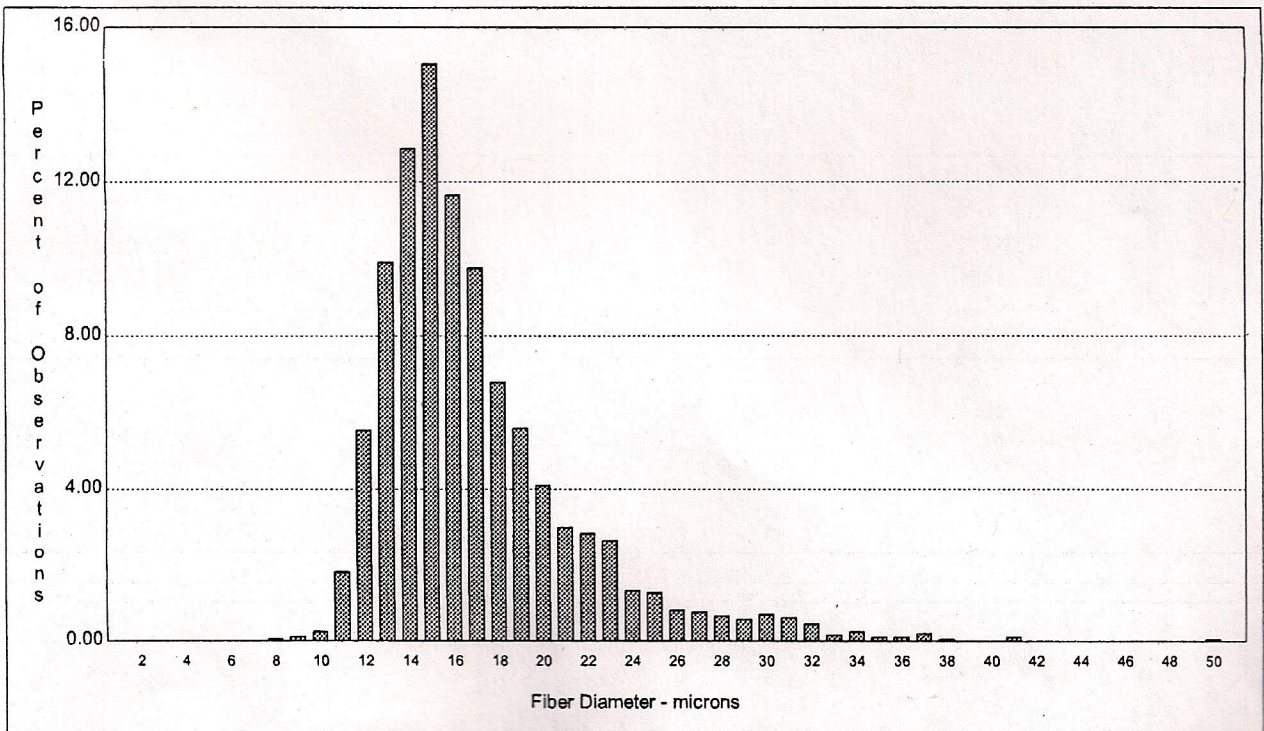

This Test Performed According to I.W.T.O Method 12