

Yocom-McColl Testing Laboratories, Inc.
 540 West Elk Place • Denver, Colorado 80216-1823 USA
 PHONE (303) 294-0582 • FAX (303) 295-6944
 EMAIL: ymccoll@ymccoll.com

**Optical Fiber Diameter Analyser (OFDA100)
 Micron Test Report**

Red Star Acres/Dwight & Marcia Andersen
 6355 Calhan Hwy
 Calhan CO 80808-9014

07/29/10


Test No: 384707

Animal and Sample Description

Animal Name: Red Star Acres Sapaccoyo Legacy I	Animal ID: Pending
Breed: Alpaca(Suri)	Sample Location: Side
Sex: Male	Sample Date: 06/11/10
Color: Beige	Age: 06/16/09

Laboratory Data

Mean Fiber Diameter: 22.8 microns	Spin Fineness: 23.0 microns
Standard Deviation: 5.7 microns	Mean Curvature (deg/mm): 10.4
Coefficient of Variation: 25.0 %	SD Curvature (deg/mm): 15.4
Fibers Greater Than 30 microns: 9.5 %	Comfort Factor: 90.5 %
Medullated Fibers: 1.6 %	

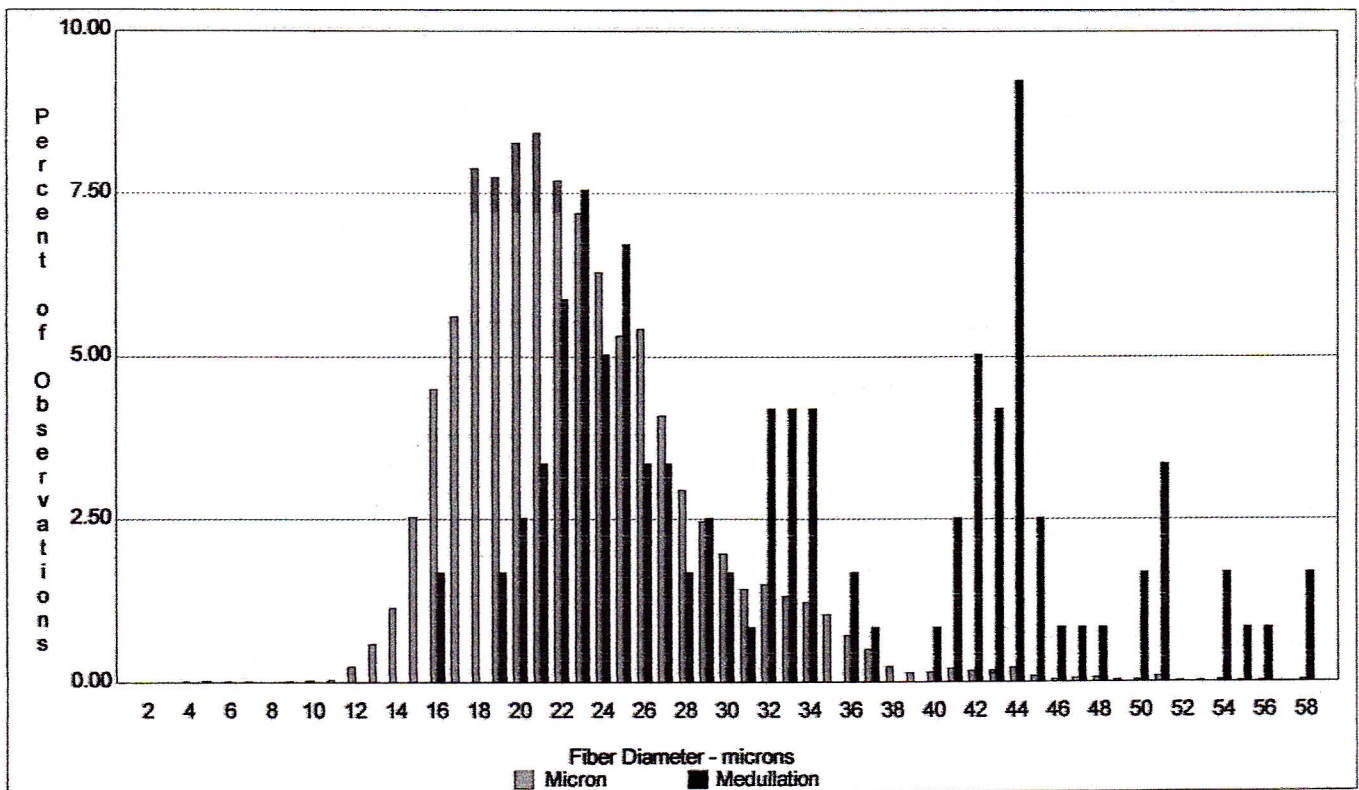

This Test Performed According to I.W.T.O Method 47