

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Flatland Ranch/Steve Trainer
21302 SW County Line Rd
Rose Hill KS 67133 USA

Date: 07/20/17

Test No: 945151


Animal and Sample Description

Animal Name: Velvet Validity
Breed: Alpaca(Huacaya)
Sex: Female
Color: Dark Brown

Animal ID: 35249788
Sample Location: Side
Sample Date: 04/24/17
Age: 05/10/14

Laboratory Data

Mean Fiber Diameter:	18.3 microns	Fibers Greater Than 30 microns:	1.3 %
Standard Deviation:	3.8 microns	Comfort Factor:	98.7 %
Coefficient of Variation:	20.8 %	Mean Curvature:	42.3 deg/mm
Spin Fineness:	17.8 microns	SD Curvature:	23.0 deg/mm

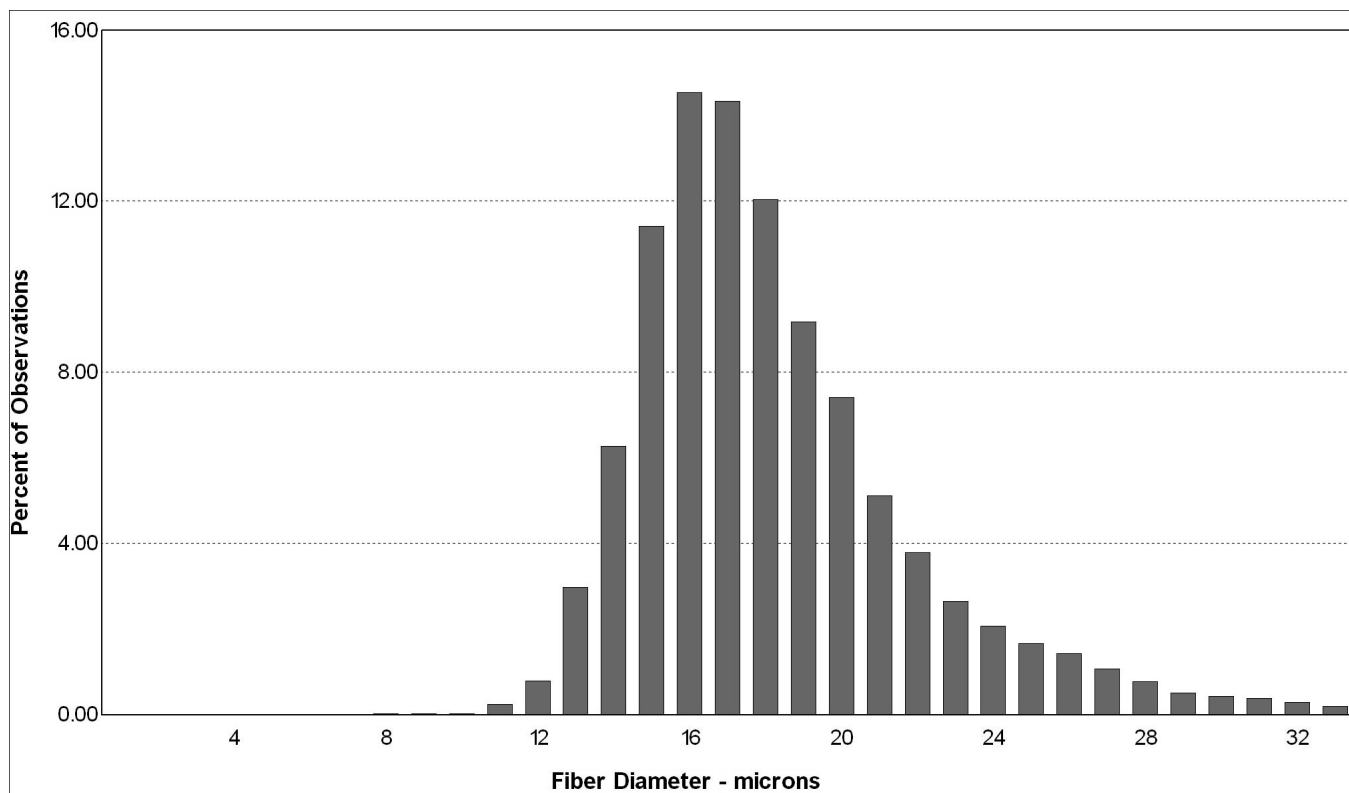

This Test Performed According to I.W.T.O Method 47