



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Thordarson Farms/Heather Thordarson
13492 S. Warnock Rd
Oregon City OR 97045 USA

Date: 07/27/16

Test No: 927873


Animal and Sample Description

Animal Name: Crown's Prince Harry
Breed: Alpaca(Huacaya)
Sex: Male
Color: Med Rose Grey

Animal ID: 32684711
Sample Location: Side
Sample Date: 06/06/16
Age: 08/18/13

Laboratory Data

Mean Fiber Diameter:	23.3 microns	Fibers Greater Than 30 microns:	8.1 %
Standard Deviation:	5.7 microns	Comfort Factor:	91.9 %
Coefficient of Variation:	24.6 %	Mean Curvature:	40.8 deg/mm
Spin Fineness:	23.4 microns	SD Curvature:	23.9 deg/mm

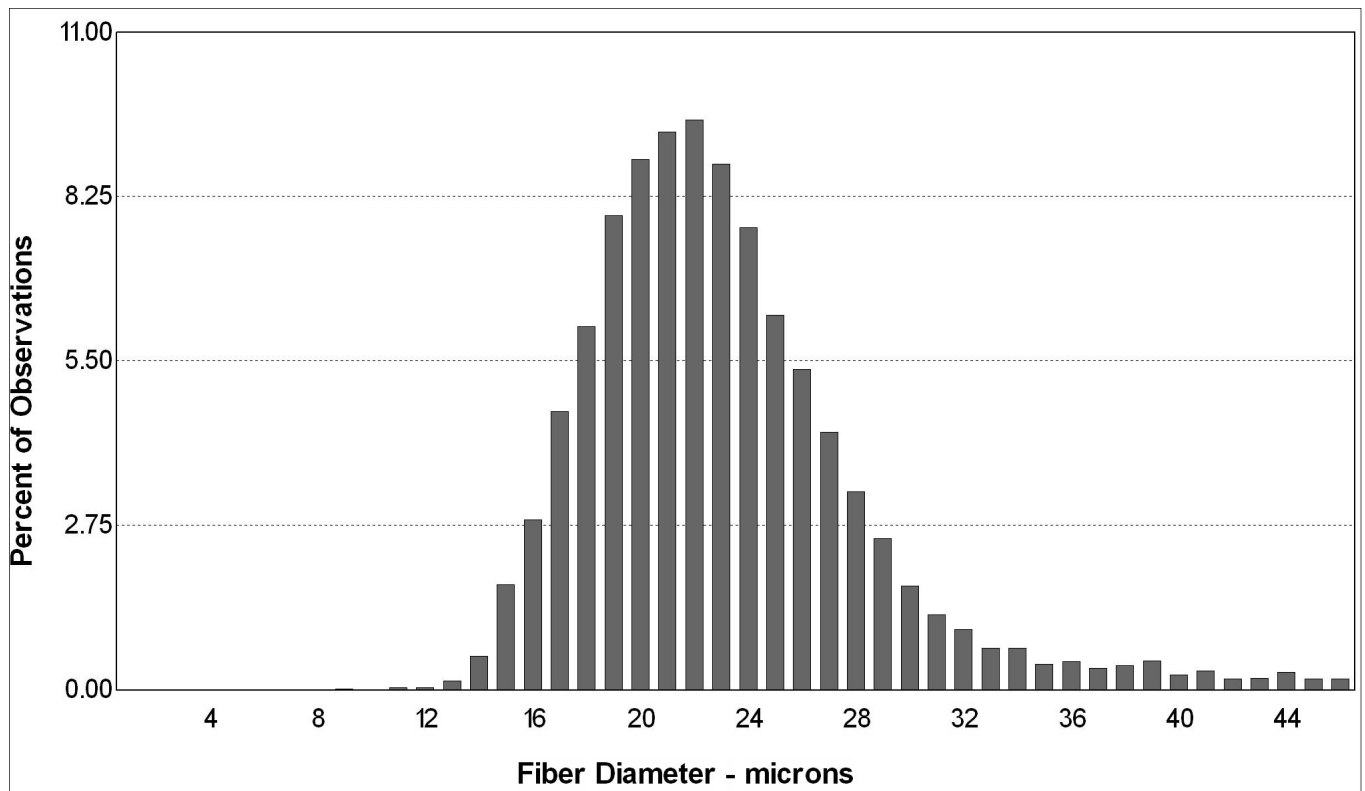

This Test Performed According to I.W.T.O Method 47