



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Thordarson Farms/Heather Thordarson
13492 S. Warnock Rd
Oregon City OR 97045 USA

Date: 07/27/16

Test No: 927878


Animal and Sample Description

Animal Name: Mountain Jewel Silver Sterling
Breed: Alpaca(Huacaya)
Sex: Male
Color: Lt Silver Grey

Animal ID: 35112693
Sample Location: Side
Sample Date: 06/06/16
Age: 08/19/14

Laboratory Data

Mean Fiber Diameter:	23.9 microns	Fibers Greater Than 30 microns:	7.1 %
Standard Deviation:	4.6 microns	Comfort Factor:	92.9 %
Coefficient of Variation:	19.1 %	Mean Curvature:	37.5 deg/mm
Spin Fineness:	22.9 microns	SD Curvature:	22.1 deg/mm

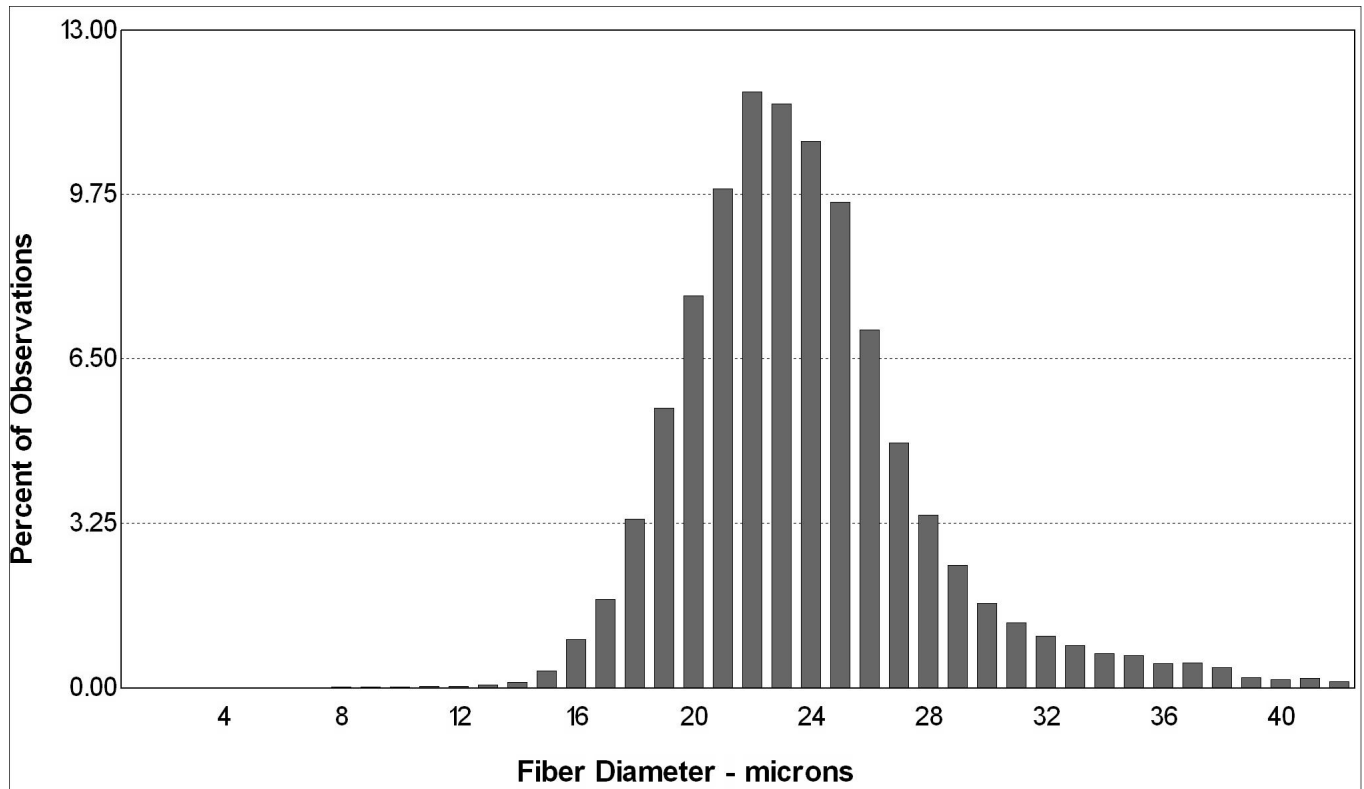

This Test Performed According to I.W.T.O Method 47