



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Cascade Rose Alpacas/Shari Hollinger
1826 324th Avenue NE
Carnation WA 98014 USA

10/11/16

Test No: 936850


Animal and Sample Description

Animal Name: Cedar Springs Sabas
Breed: Alpaca(Huacaya)
Sex: Male
Color: Med Silver Grey

Animal ID: 31533904
Sample Location: Mid Side
Sample Date: 05/31/16
Age: 08/03/11

Laboratory Data

Mean Fiber Diameter:	25.2 microns	Spin Fineness:	24.8 microns
Standard Deviation:	5.6 microns	Mean Curvature (deg/mm):	35.1
Coefficient of Variation:	22.0 %	SD Curvature (deg/mm):	21.2
Fibers Greater Than 30 microns:	14.5 %	Comfort Factor:	85.5 %

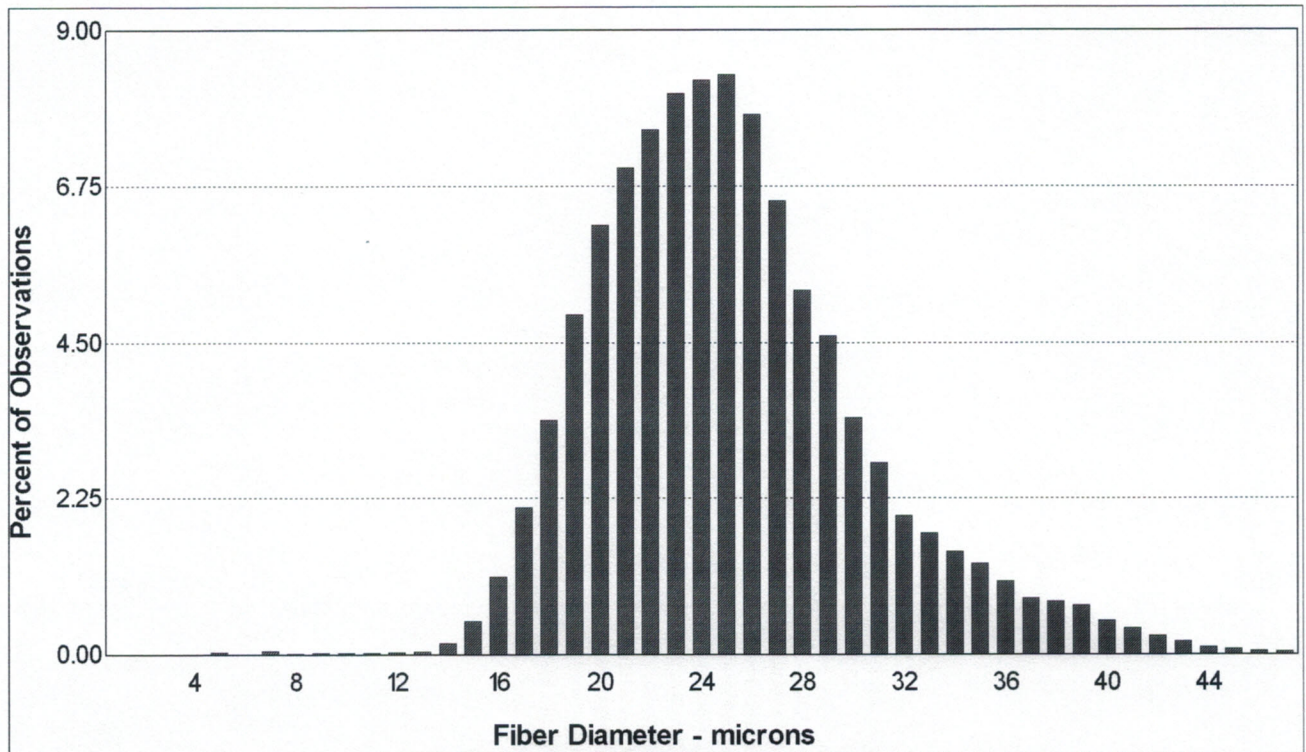

This Test Performed According to I.W.T.O Method 47