



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Cascade Rose Alpacas/Shari Hollinger  
1826 324th Avenue NE  
Carnation WA 98014 USA

**Date:** 09/27/16  
**Shear ID:** 133958  
**Test No:** 935044


### Animal and Sample Description

**Animal Name:** Picchu Dot  
**ARI #:** 32278910  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Lt Silver Grey

**Date of Birth (Age):** 07/11/14  
**Sample Location:** Side  
**Sample Date:** 05/31/16  
**Previous Shear Date:** 05/28/15  
**Total Fleece Wt (lbs):** 5.90

### Laboratory Data

<b>Mean Fiber Diameter:</b>	23.1 microns	<b>Mean Staple Length:</b>	101.8 mm
<b>Standard Deviation:</b>	5.7 microns	<b>Length Standard Deviation:</b>	5.8 mm
<b>Coefficient of Variation:</b>	24.6 %	<b>Length Coefficient of Variation:</b>	5.7 %
<b>Spin Fineness:</b>	23.3 microns	<b>Mean Curvature:</b>	36.9 deg/mm
<b>Fibers Greater Than 30 microns:</b>	9.0 %	<b>SD Curvature:</b>	21.8 deg/mm
<b>Comfort Factor:</b>	91.0 %		

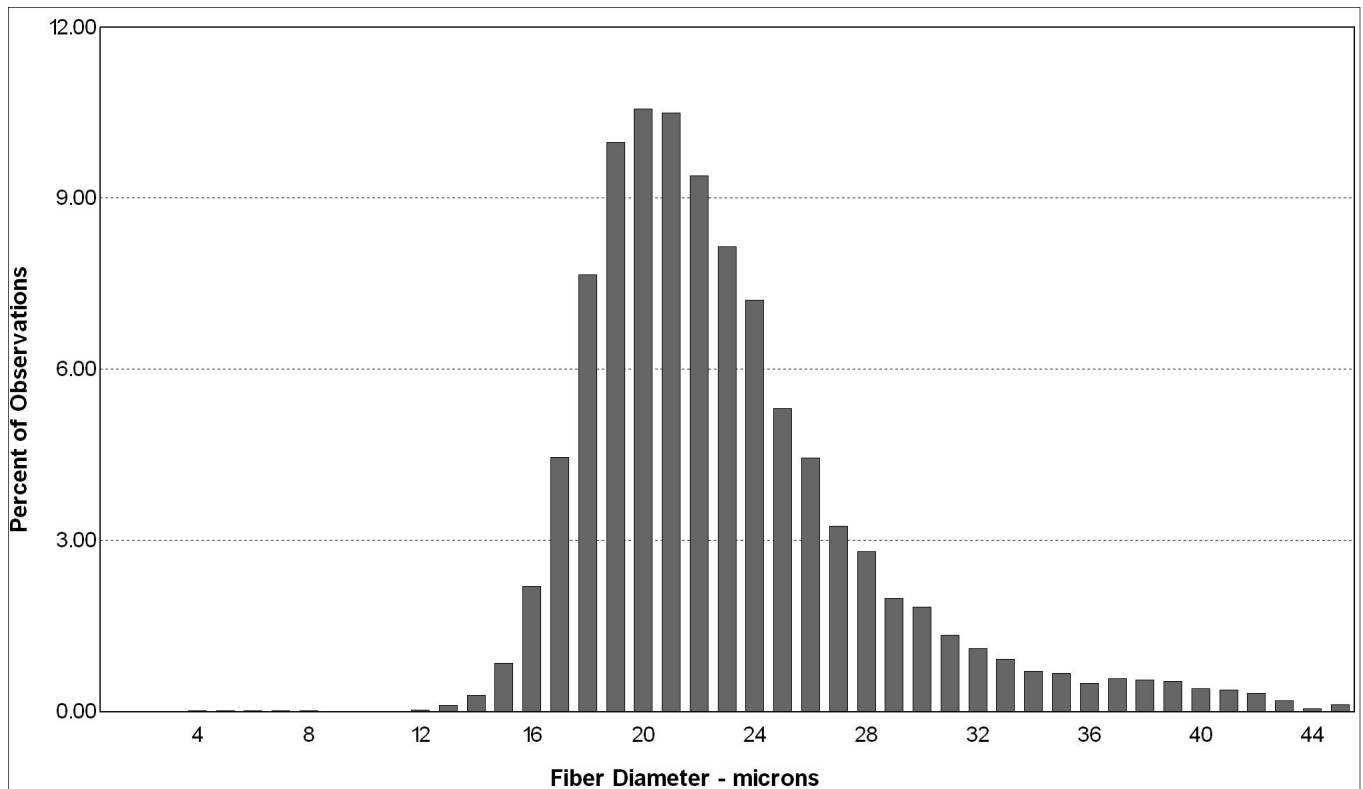

This Test Performed According to I.W.T.O Method 47