



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Alpaca Palace LLC/Renee A Ritenour  
102 Knotingham Lane  
Butler PA 16001

05/22/18

Test No: 959678


### Animal and Sample Description

**Animal Name:** Alpaca Palace Captain's First Mate  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** Dark Fawn

**Animal ID:** 35401285  
**Sample Location:** Side (R)  
**Sample Date:** 05/05/18  
**Age:** 05/16/17

### Laboratory Data

**Mean Fiber Diameter:** 13.2 microns  
**Standard Deviation:** 2.8 microns  
**Coefficient of Variation:** 21.0 %  
**Fibers Greater Than 30 microns:** 0.0 %

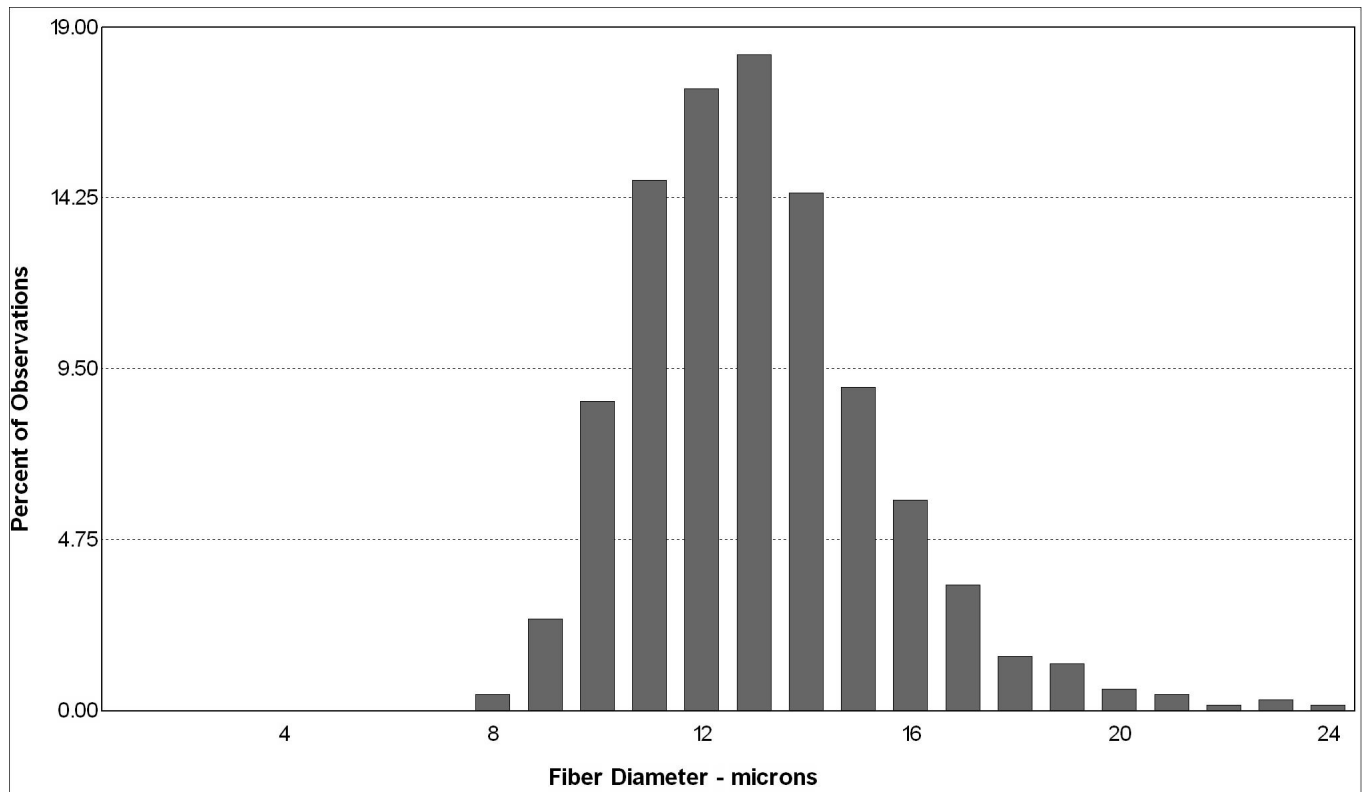

This Test Performed According to I.W.T.O Method 12