



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Alpaca Palace LLC/Renee A Ritenour
102 Knotingham Lane
Butler PA 16001

08/14/17


Test No: 942216

Animal and Sample Description

Animal Name:	Alpaca Palace Crown's Gypsy Rose	Animal ID:	32048063
Breed:	Alpaca(Huacaya)	Sample Location:	Side (R)
Sex:	Female	Sample Date:	05/07/17
Color:	Bay Black 985141000544088	Age:	07/27/11

Laboratory Data

Mean Fiber Diameter:	20.2 microns
Standard Deviation:	4.2 microns
Coefficient of Variation:	21.0 %
Fibers Greater Than 30 microns:	2.5 %

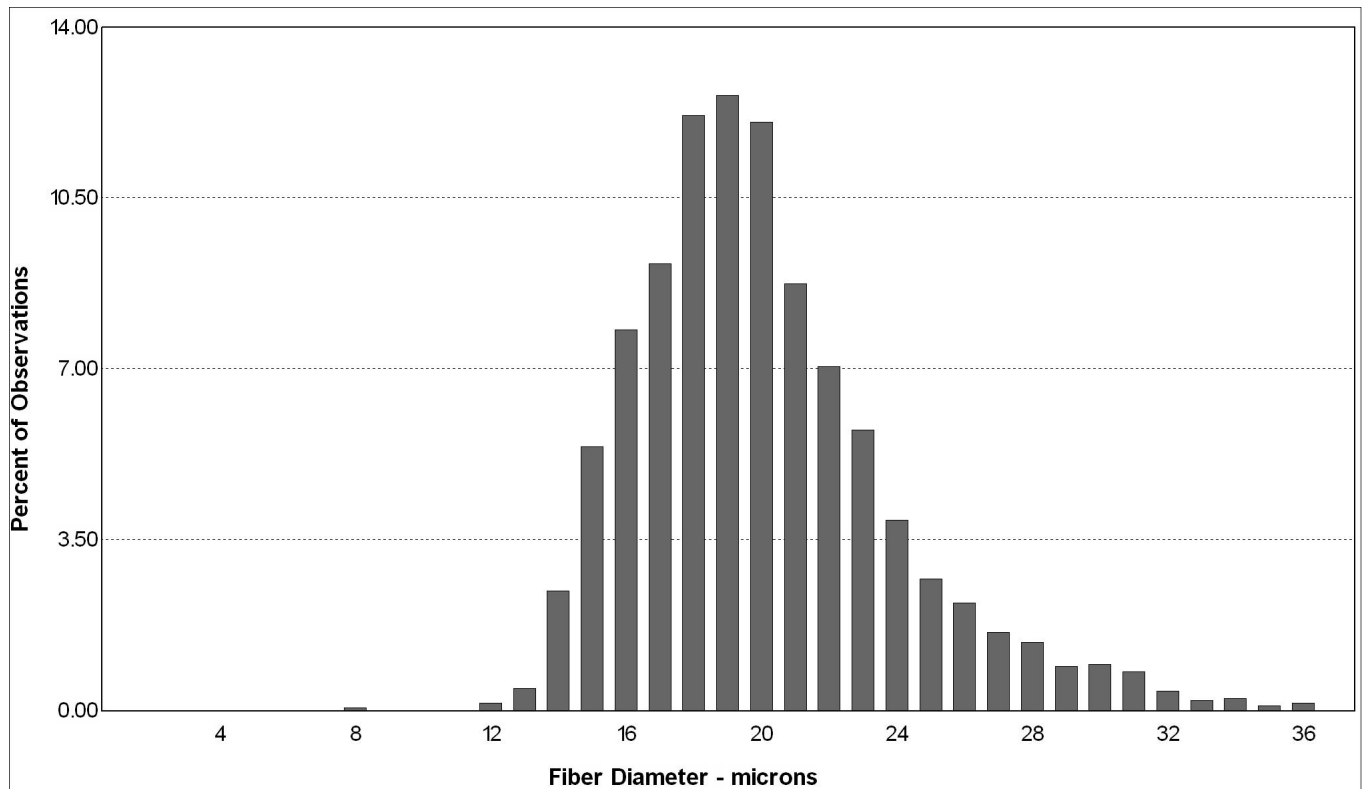

This Test Performed According to I.W.T.O Method 12