



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Alpaca Palace LLC/Renee A Ritenour  
102 Knotingham Lane  
Butler PA 16001

08/14/17

Test No: 942172


### Animal and Sample Description

**Animal Name:** Alpaca Palace Houdini's Harmony  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Med Fawn 985141000544064

**Animal ID:** 32574838  
**Sample Location:** Side (R)  
**Sample Date:** 05/07/17  
**Age:** 05/13/13

### Laboratory Data

**Mean Fiber Diameter:** 20.2 microns  
**Standard Deviation:** 4.8 microns  
**Coefficient of Variation:** 23.7 %  
**Fibers Greater Than 30 microns:** 3.7 %

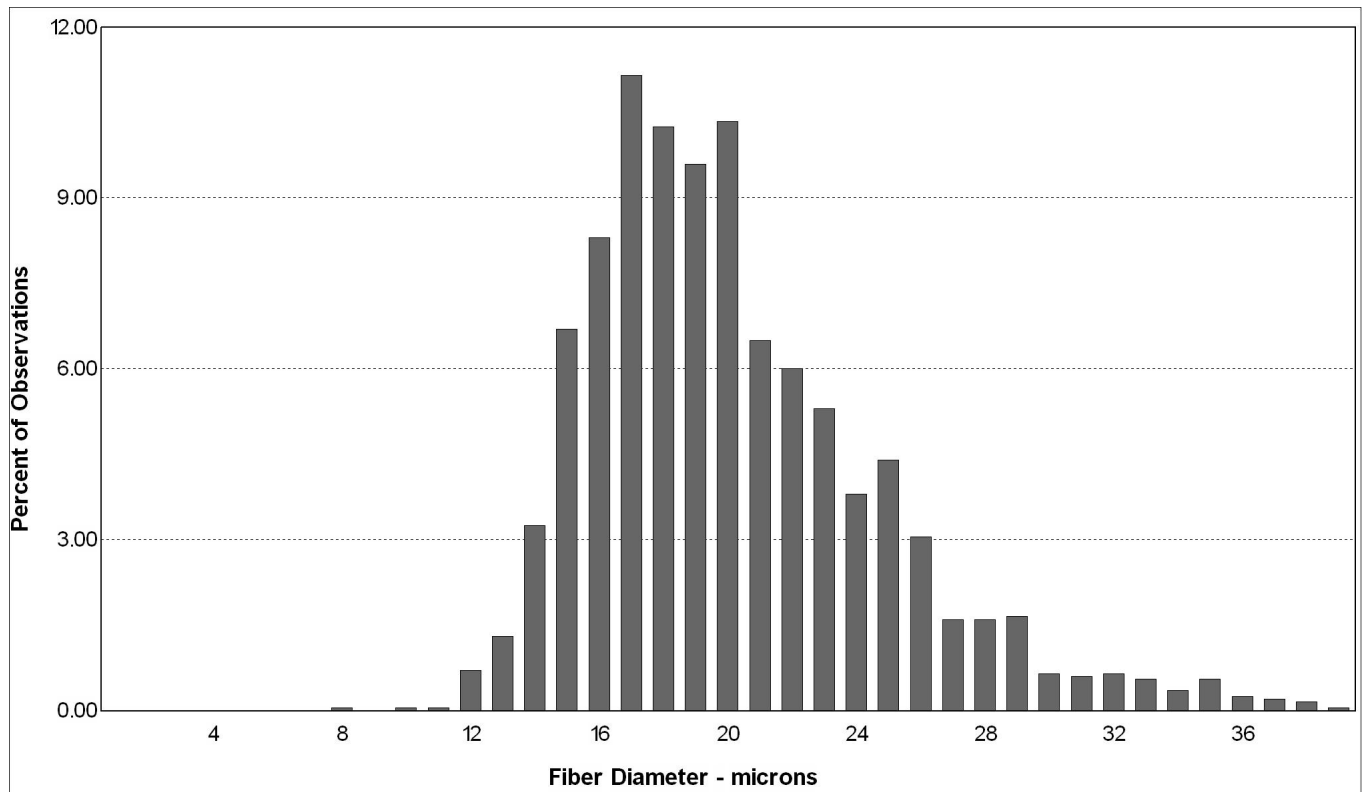

This Test Performed According to I.W.T.O Method 12