



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Alpaca Palace LLC/Renee A Ritenour  
102 Knotingham Lane  
Butler PA 16001

05/22/18

**Test No:** 959734


### Animal and Sample Description

**Animal Name:** Alpaca Palace Zagato' Jolene  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Dark Rose Grey

**Animal ID:** 35401384  
**Sample Location:** Side (R)  
**Sample Date:** 05/05/18  
**Age:** 08/05/17

### Laboratory Data

**Mean Fiber Diameter:** 15.1 microns  
**Standard Deviation:** 2.8 microns  
**Coefficient of Variation:** 18.5 %  
**Fibers Greater Than 30 microns:** 0.3 %

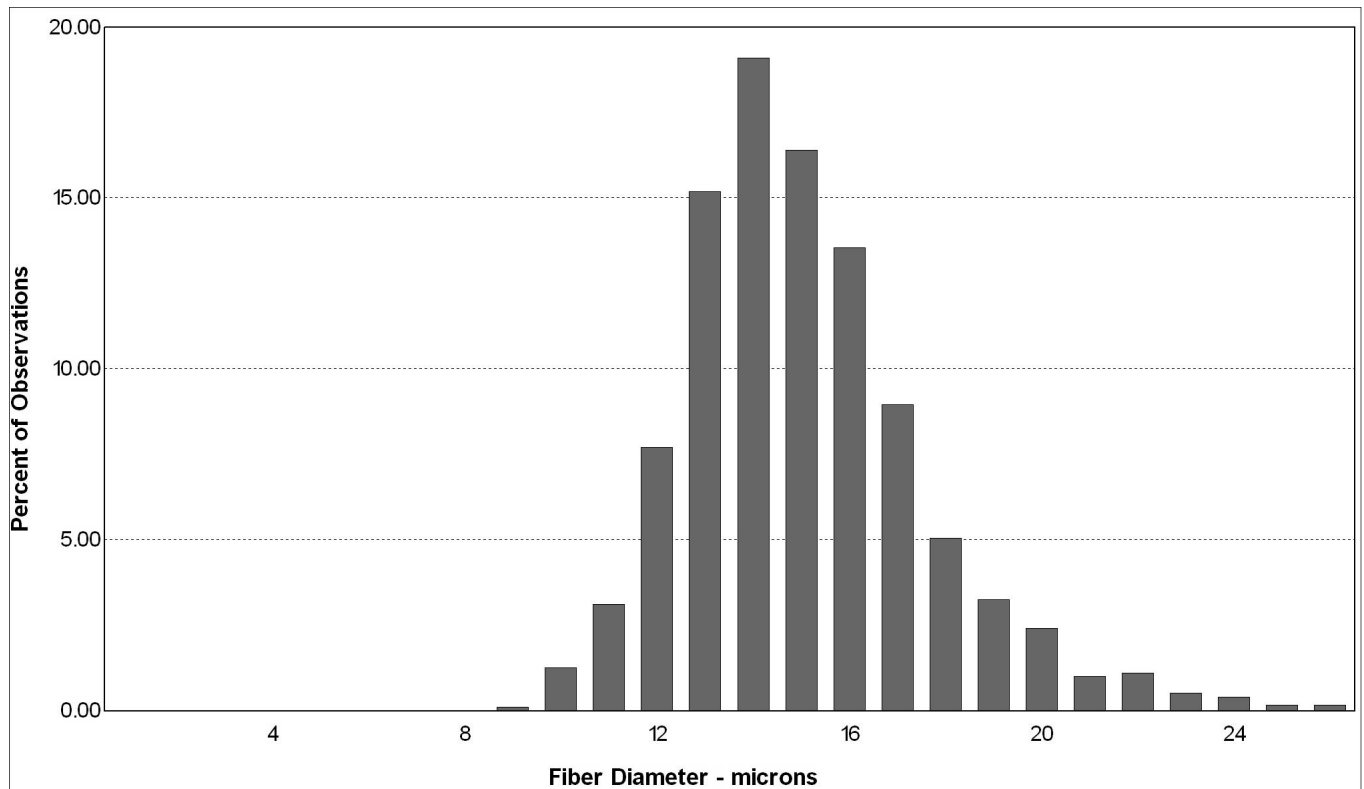

This Test Performed According to I.W.T.O Method 12