



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Serenity at Stony Point/Valerie Chavez
226 Walker Valley Dr
Stony Point NC 28678-9232 USA

04/28/17

Test No: 940979


Animal and Sample Description

Animal Name: CFI Peruvian Desiree
Breed: Alpaca(Huacaya)
Sex: Female
Color: Med Fawn

Animal ID: 35041962
Sample Location: Side (L)
Sample Date: 04/07/17
Age: 06/08/15

Laboratory Data

Mean Fiber Diameter: 15.9 microns
Standard Deviation: 4.5 microns
Coefficient of Variation: 28.2 %
Fibers Greater Than 30 microns: 1.1 %

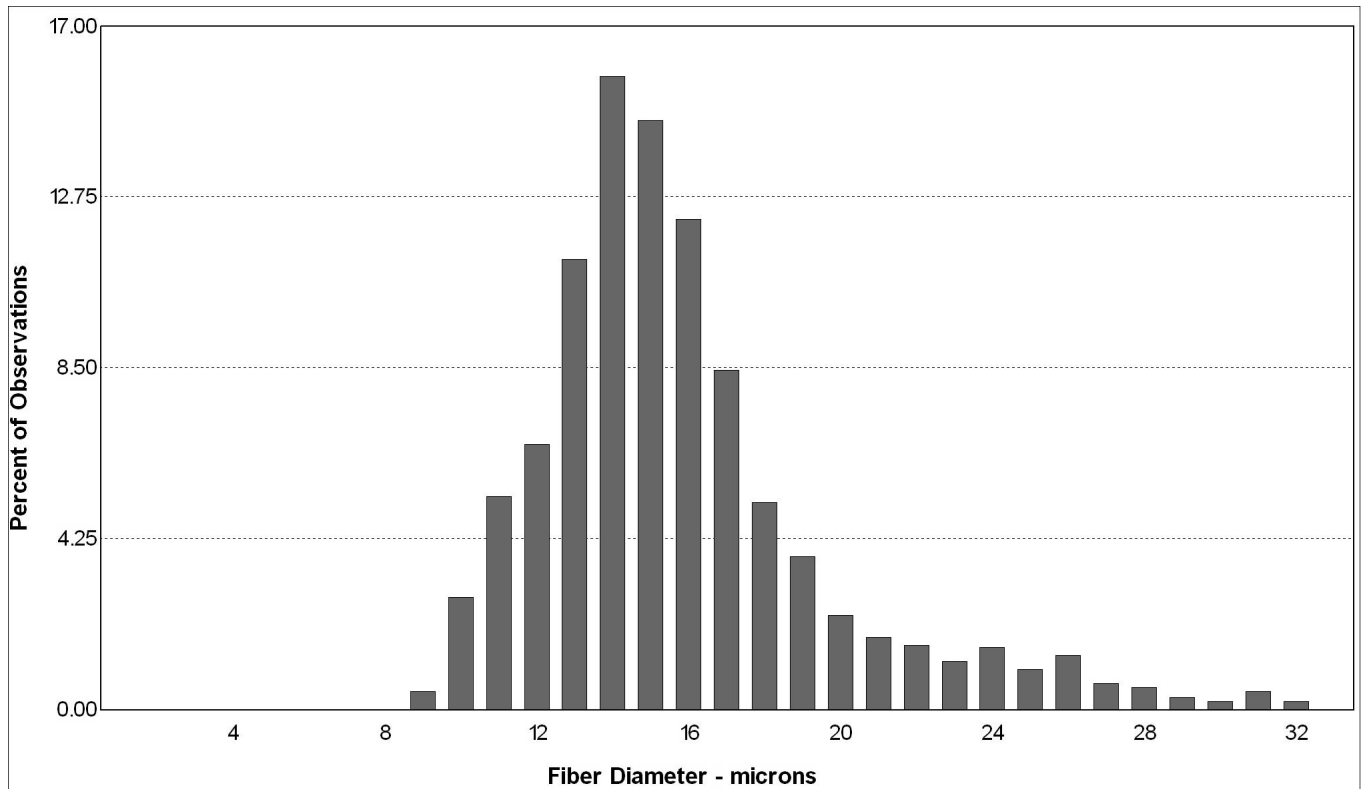

This Test Performed According to I.W.T.O Method 12