



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Serenity at Stony Point/Valerie Chavez
226 Walker Valley Dr
Stony Point NC 28678-9232 USA

04/28/17

Test No: 940976


Animal and Sample Description

Animal Name: CFI Peruvian Xenos's Xena
Breed: Alpaca(Huacaya)
Sex: Female
Color: Lt Fawn

Animal ID: 35066422
Sample Location: Side (L)
Sample Date: 04/07/17
Age: 06/23/14

Laboratory Data

Mean Fiber Diameter: 23.3 microns
Standard Deviation: 4.4 microns
Coefficient of Variation: 18.9 %
Fibers Greater Than 30 microns: 5.3 %

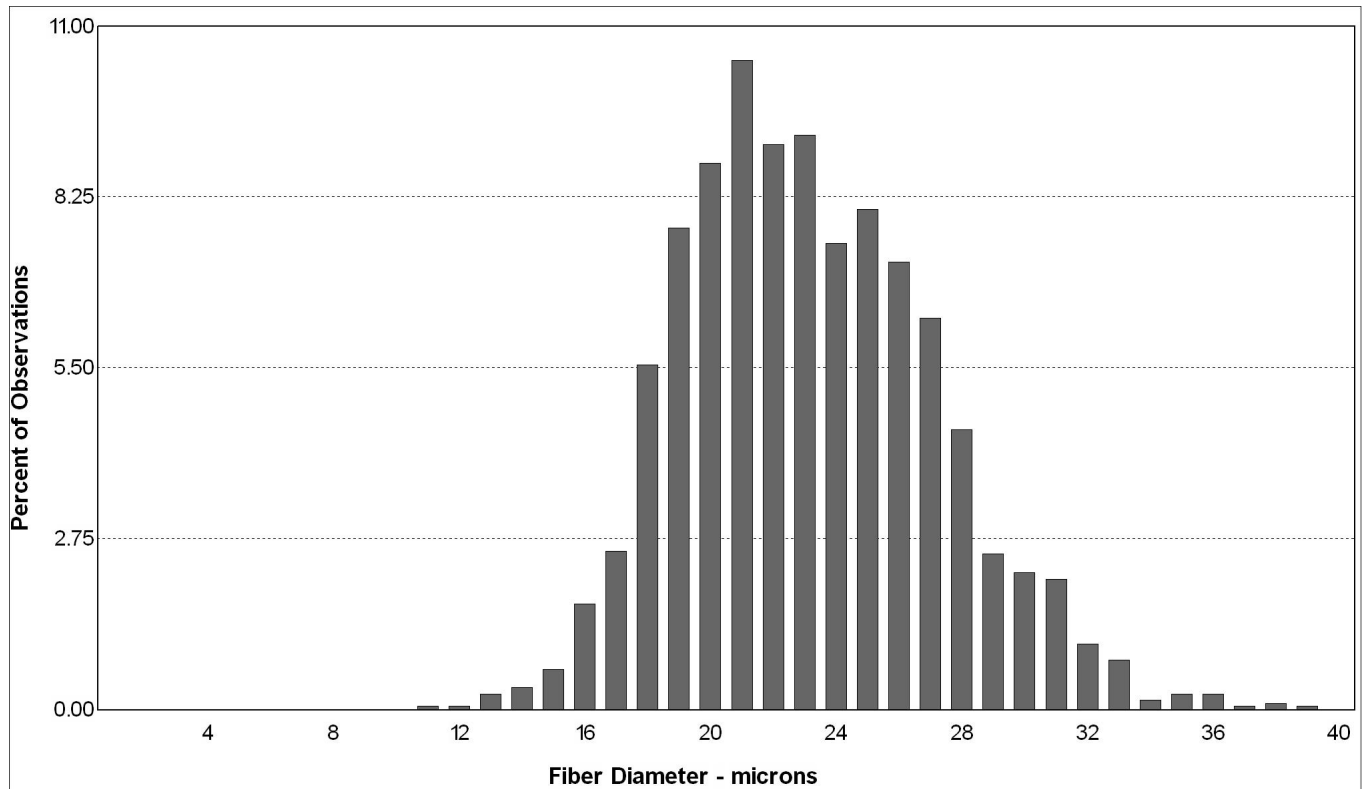

This Test Performed According to I.W.T.O Method 12