



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Serenity at Stony Point/Valerie Stevens  
226 Walker Valley Dr  
Stony Point NC 28678 USA

04/22/16

Test No: 920176


### Animal and Sample Description

**Animal Name:** Cleo's Kuhl Spot  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** White/Fawn (Appy)

**Animal ID:** 35278467  
**Sample Location:** Side (R)  
**Sample Date:** 04/06/16  
**Age:** 07/22/14

### Laboratory Data

**Mean Fiber Diameter:** 19.9 microns  
**Standard Deviation:** 3.7 microns  
**Coefficient of Variation:** 18.5 %  
**Fibers Greater Than 30 microns:** 1.3 %

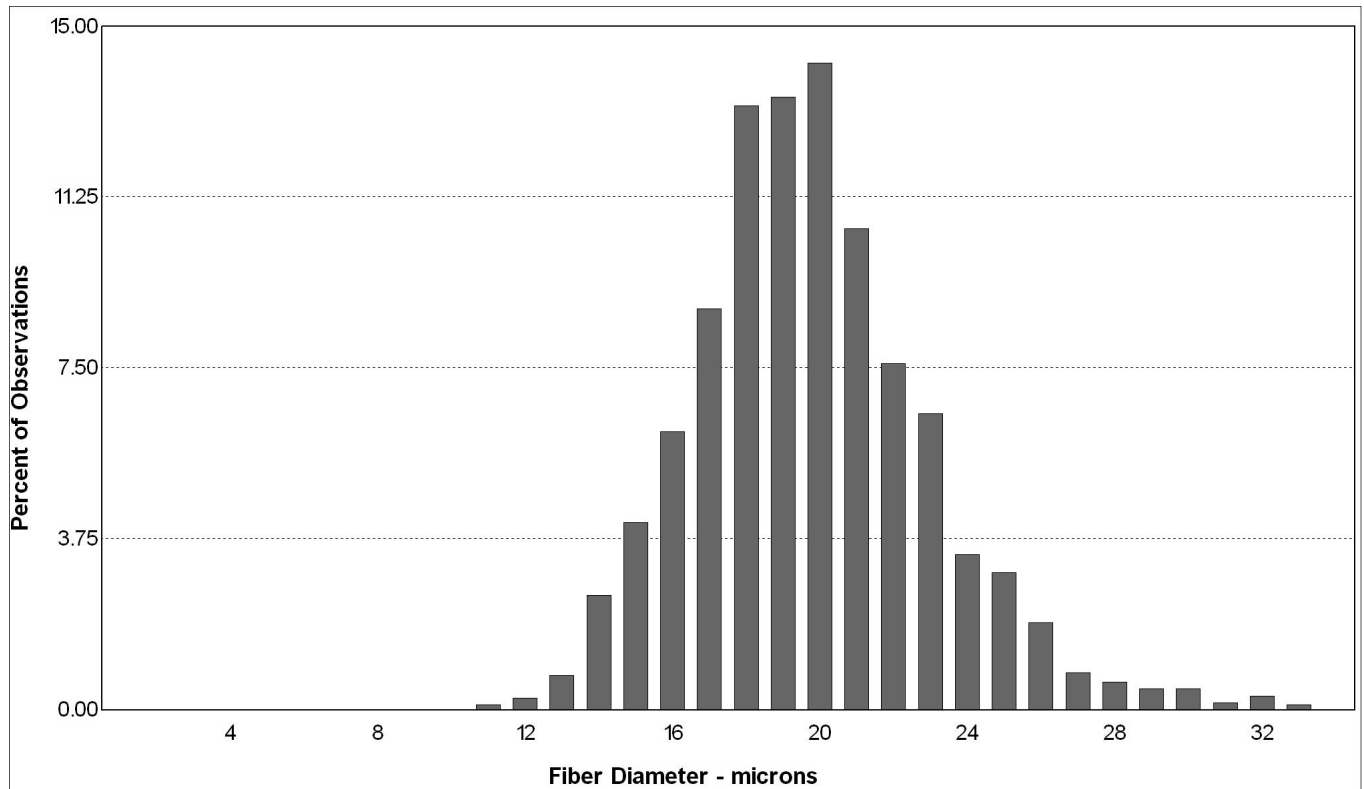

This Test Performed According to I.W.T.O Method 12