



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Harley Hill Farm LLC/William Oraschin  
451 Kellers Road  
Quakertown PA 18951 USA

**Date:** 03/14/17

**Test No:** 939662


### Animal and Sample Description

**Animal Name:** Harley Carmel Candy  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Med Fawn

**Animal ID:** 32697971  
**Sample Location:** Side (L)  
**Sample Date:** 03/08/17  
**Age:** 09/22/16

### Laboratory Data

<b>Mean Fiber Diameter:</b>	17.0 microns	<b>Fibers Greater Than 30 microns:</b>	0.3 %
<b>Standard Deviation:</b>	3.1 microns	<b>Comfort Factor:</b>	99.7 %
<b>Coefficient of Variation:</b>	18.0 %	<b>Mean Curvature:</b>	36.1 deg/mm
<b>Spin Fineness:</b>	16.1 microns	<b>SD Curvature:</b>	25.2 deg/mm

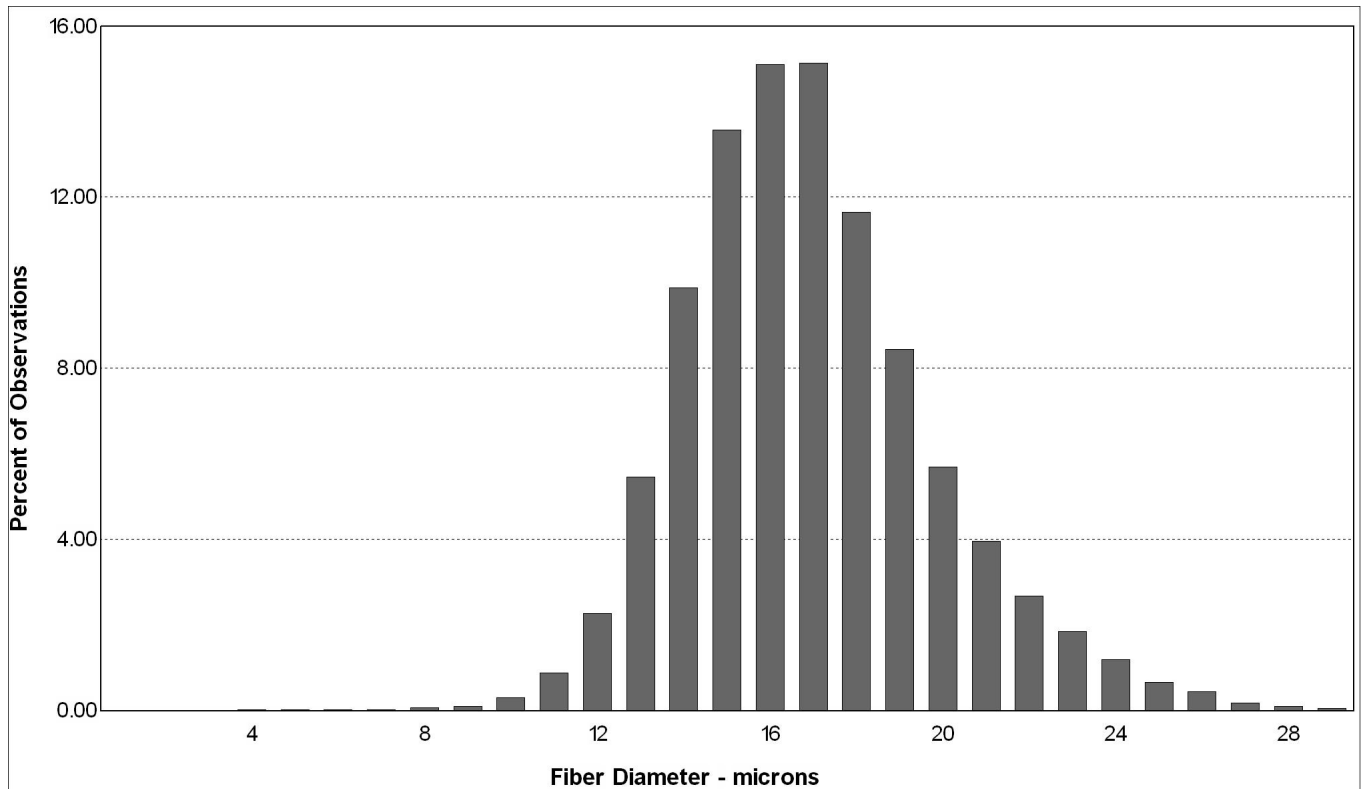

This Test Performed According to I.W.T.O Method 47