



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Nite Star Alpacas/Ann Nogier
1301 Larson Rd
Schwenksville PA 19473 USA

Date: 05/02/18

Test No: 958524


Animal and Sample Description

Animal Name: Zander
Breed: Alpaca(Huacaya)
Sex: Male
Color: Dark Grey

Animal ID: XXXXX
Sample Location: Side (L)
Sample Date: 04/21/18
Age: 05/10/17

Laboratory Data

Mean Fiber Diameter:	21.8 microns	Fibers Greater Than 30 microns:	3.3 %
Standard Deviation:	4.3 microns	Comfort Factor:	96.7 %
Coefficient of Variation:	19.7 %	Mean Curvature:	35.0 deg/mm
Spin Fineness:	21.0 microns	SD Curvature:	20.7 deg/mm

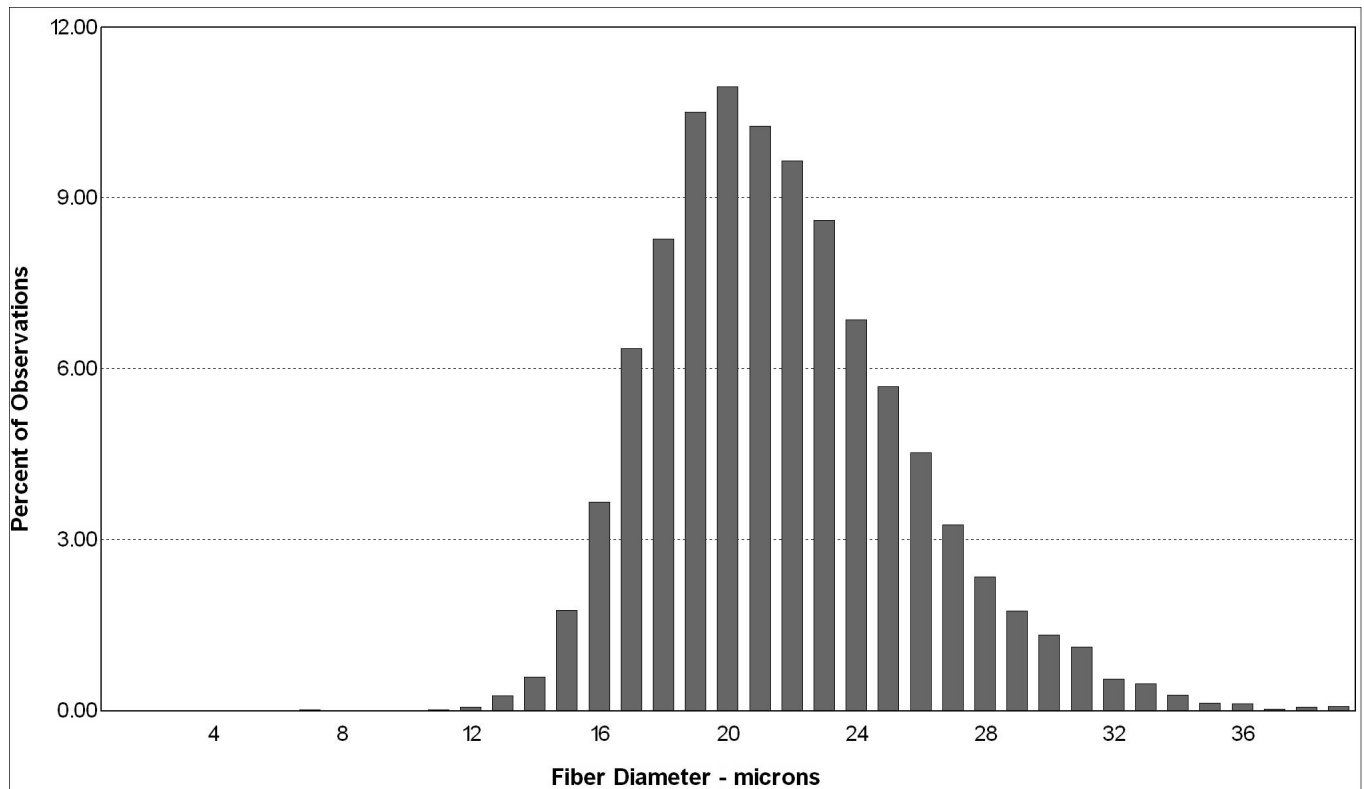

This Test Performed According to I.W.T.O Method 47