



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Shiloh Springs Ranch/Nancy Masak
39505 Avenida Bonita
Murrieta CA 92562

Date: 04/27/17

Test No: 940945


Animal and Sample Description

Animal Name: Luzie Luna of Bright Water
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 32572797
Sample Location: Side (L)
Sample Date: 04/07/17
Age: 05/21/12

Laboratory Data

Mean Fiber Diameter:	24.7 microns	Fibers Greater Than 30 microns:	14.8 %
Standard Deviation:	5.3 microns	Comfort Factor:	85.2 %
Coefficient of Variation:	21.6 %	Mean Curvature:	44.0 deg/mm
Spin Fineness:	24.1 microns	SD Curvature:	31.4 deg/mm

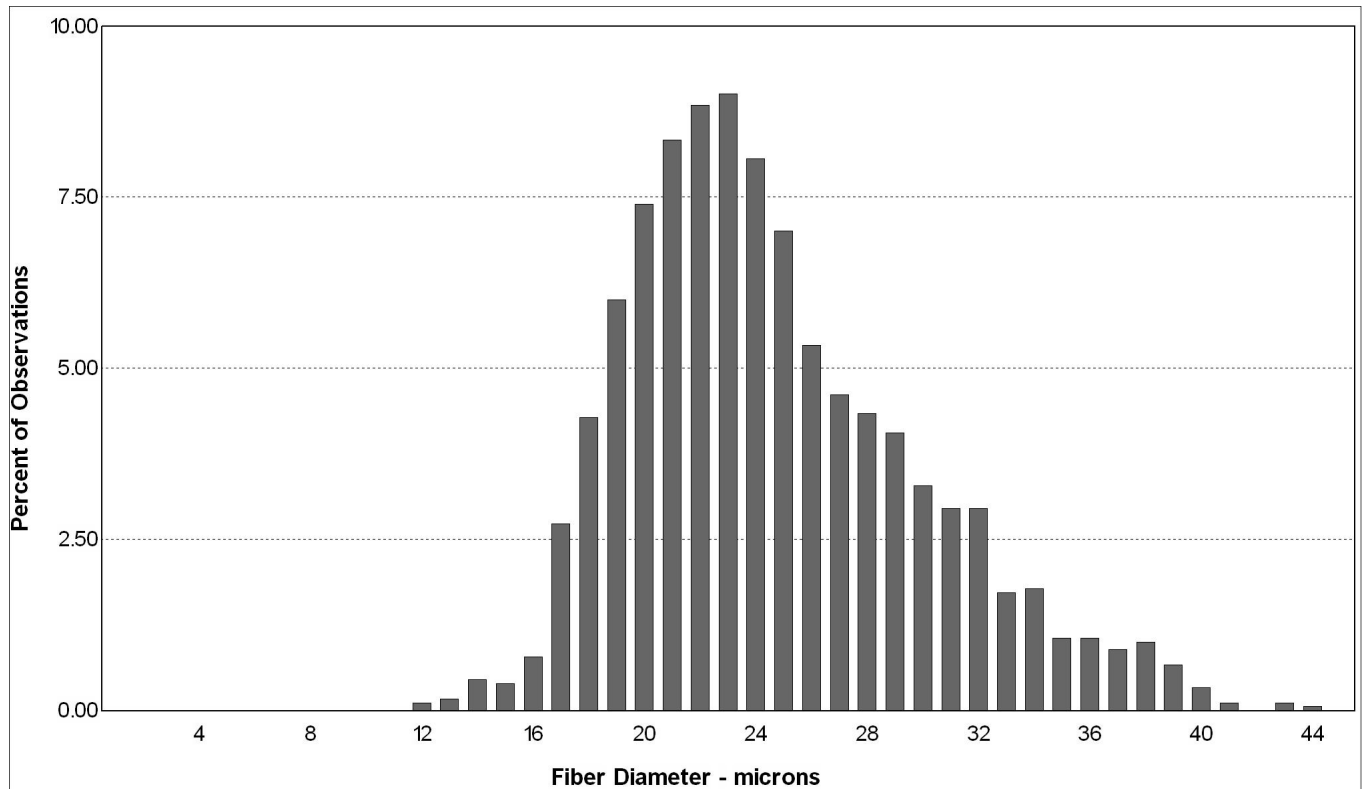

This Test Performed According to I.W.T.O Method 47