

Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

**Sirolan Laserscan
Micron Test Report**

Kendall Creek Farms/Chris & Lori Works
41 Looker Mountain Trail
Bradford PA 16701 USA

08/04/14

Test No: 488308


Animal and Sample Description

Animal Name: KCF Peruvian Shelby
Breed: Alpaca(Huacaya)
Sex: Male
Color: WH

Animal ID: 32438611
Sample Location: Side (L)
Sample Date: 05/15/14
Age: 10/05/11

Laboratory Data

Mean Fiber Diameter: 20.6 microns
Standard Deviation: 4.2 microns
Coefficient of Variation: 20.6 %
Fibers Greater Than 30 microns: 2.6 %

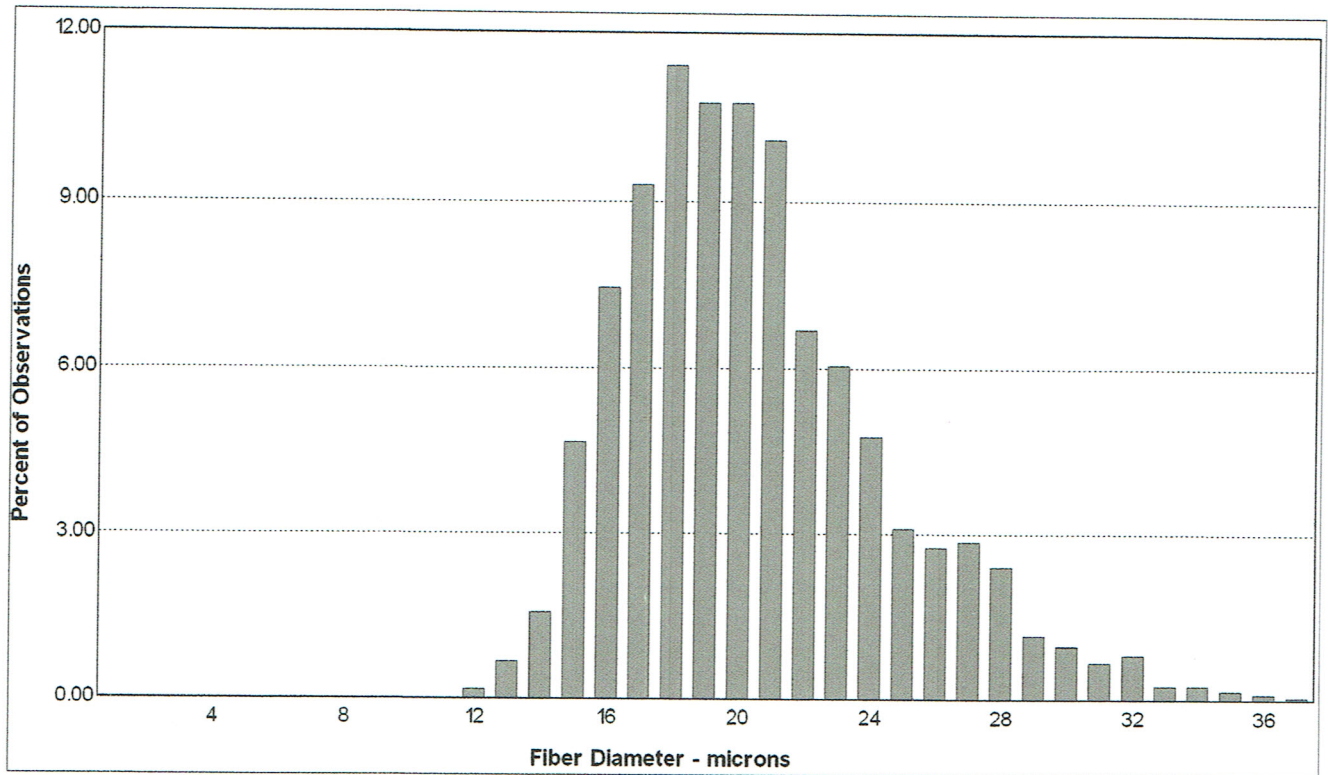

This Test Performed According to I.W.T.O Method 12