

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Crescent Moon Ranch/Scott Miller
70397 Buckhorn Road
Terrebonne OR 97760 U.S.A.

07/29/08

Test No: 331814


Animal and Sample Description

Animal Name: Crescent Moon's Sixtus
Breed: Alpaca(Huacaya)
Sex: Male
Color: BB

Animal ID: 30842595
Sample Location: Blanket
Sample Date: 06/01/08
Age: 06/09/07

Laboratory Data

Mean Fiber Diameter: 19.7 microns
Standard Deviation: 4.6 microns
Coefficient of Variation: 23.4 %
Fibers Greater Than 30 microns: 2.2 %

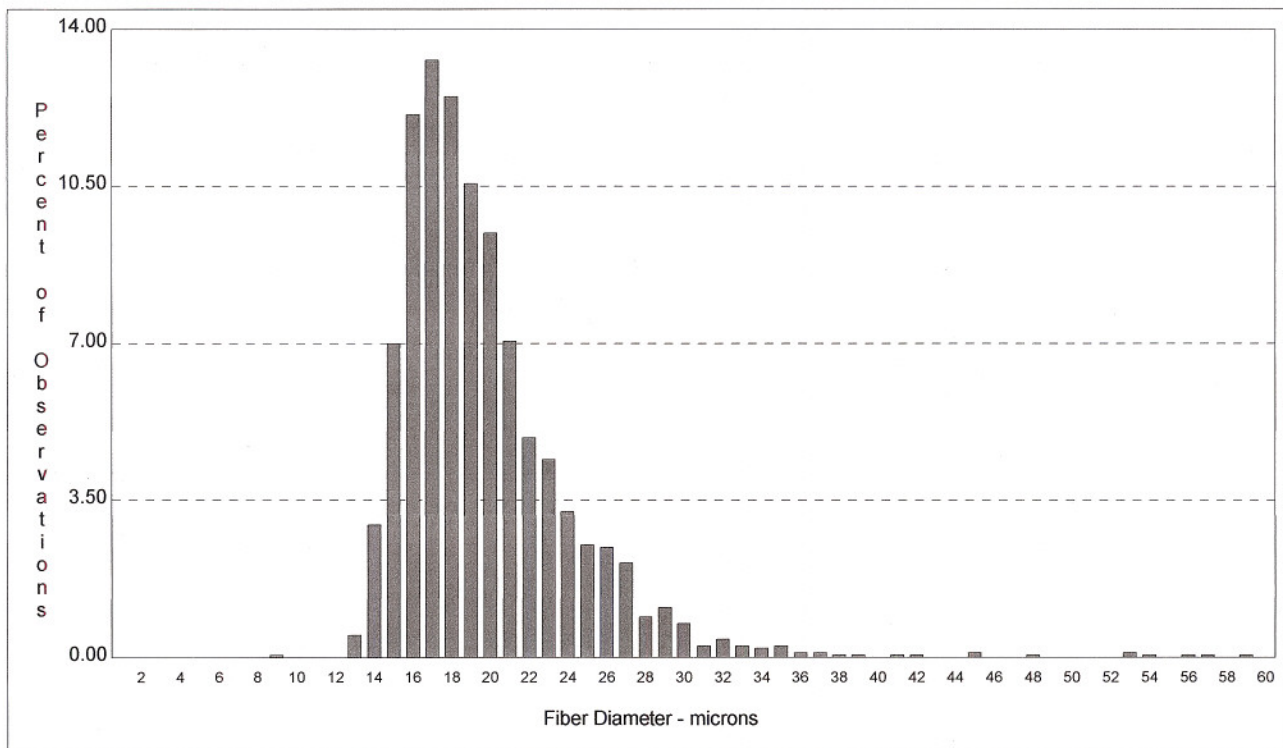

This Test Performed According to I.W.T.O Method 12



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Crescent Moon Ranch/Scott Miller
70397 Buckhorn Road
Terrebonne OR 97760 U.S.A.

08/03/09

Test No: 360178


Animal and Sample Description

Animal Name: Crescent Moon's Sixtus
Breed: Alpaca(Huacaya)
Sex: Male
Color: BB

Animal ID: 30842595
Sample Location: Blanket
Sample Date: 06/30/09
Age: 06/09/07

Laboratory Data

Mean Fiber Diameter: 23.4 microns
Standard Deviation: 3.9 microns
Coefficient of Variation: 16.9 %
Fibers Greater Than 30 microns: 5.1 %

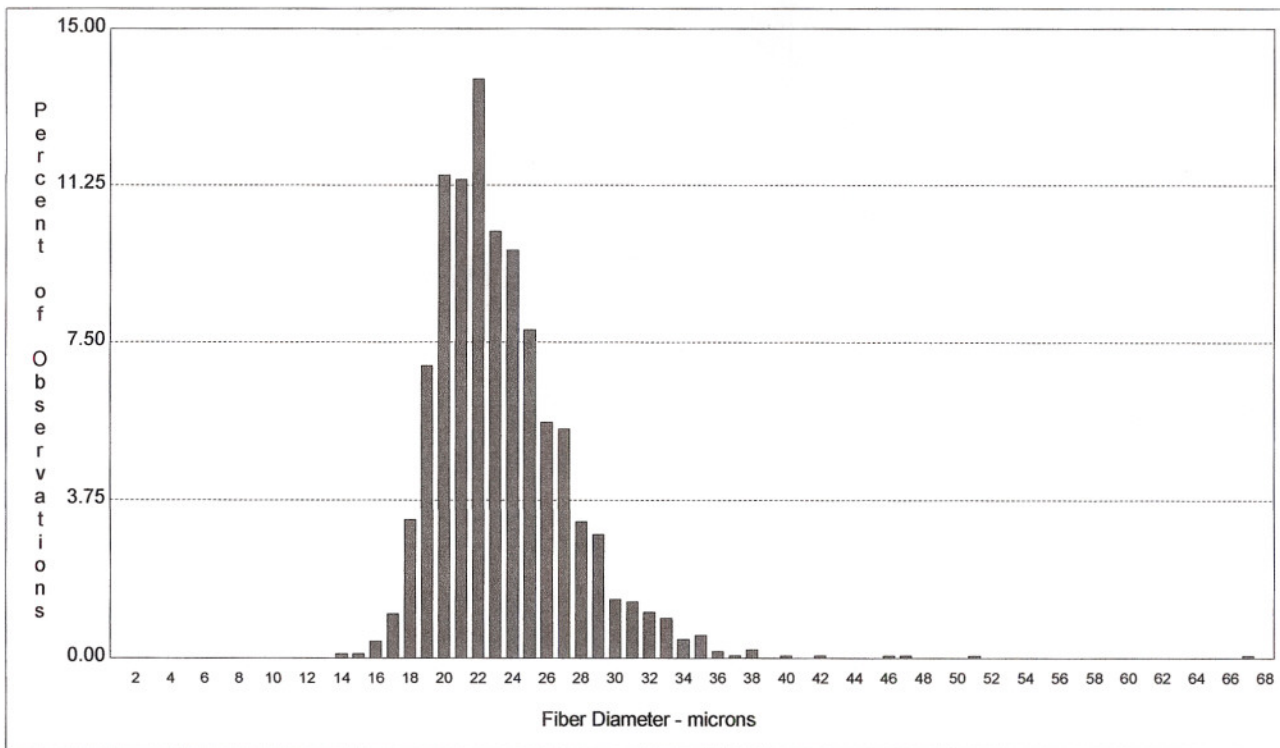

This Test Performed According to I.W.T.O Method 12



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Crescent Moon Ranch/Scott Miller
70397 Buckhorn Road
Terrebonne OR 97760 U.S.A.

06/17/10

Test No: 377906


Animal and Sample Description

Animal Name: Crescent Moon's Sixtus
Breed: Alpaca(Huacaya)
Sex: Male
Color: Bay Black

Animal ID: 30842595
Sample Location: Blanket
Sample Date: 06/03/10
Age: 06/09/07

Laboratory Data

Mean Fiber Diameter: 24.4 microns
Standard Deviation: 4.1 microns
Coefficient of Variation: 16.8 %
Fibers Greater Than 30 microns: 8.0 %

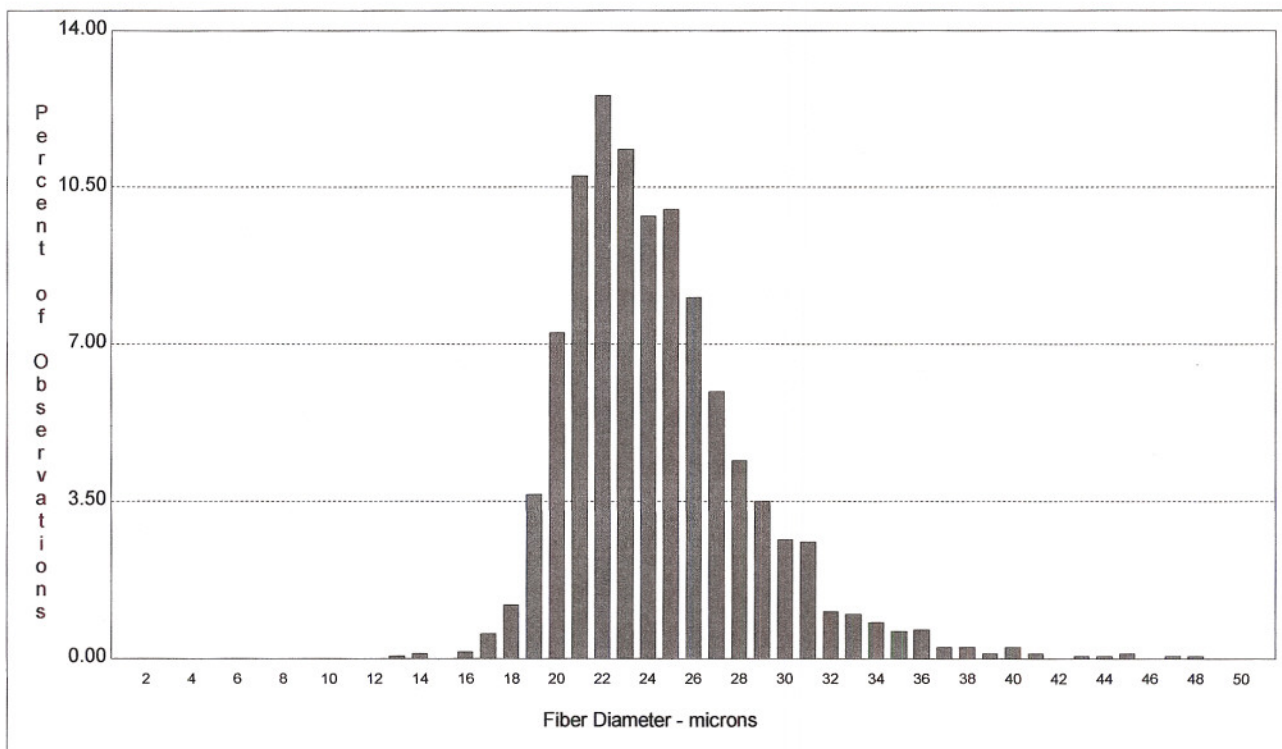

This Test Performed According to I.W.T.O Method 12