

Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

**Sirolan Laserscan
Micron Test Report**

R & R Ranch/Richard & Robin Vasquez
325B Denio Avenue
Gilroy CA 95020-9203 USA

07/19/10

Test No: 384066


Animal and Sample Description

Animal Name: Apple
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 30580244
Sample Location: Side
Sample Date: 06/03/10
Age: 07/29/07

Laboratory Data

Mean Fiber Diameter: 24.8 microns
Standard Deviation: 4.9 microns
Coefficient of Variation: 19.6 %
Fibers Greater Than 30 microns: 10.1 %

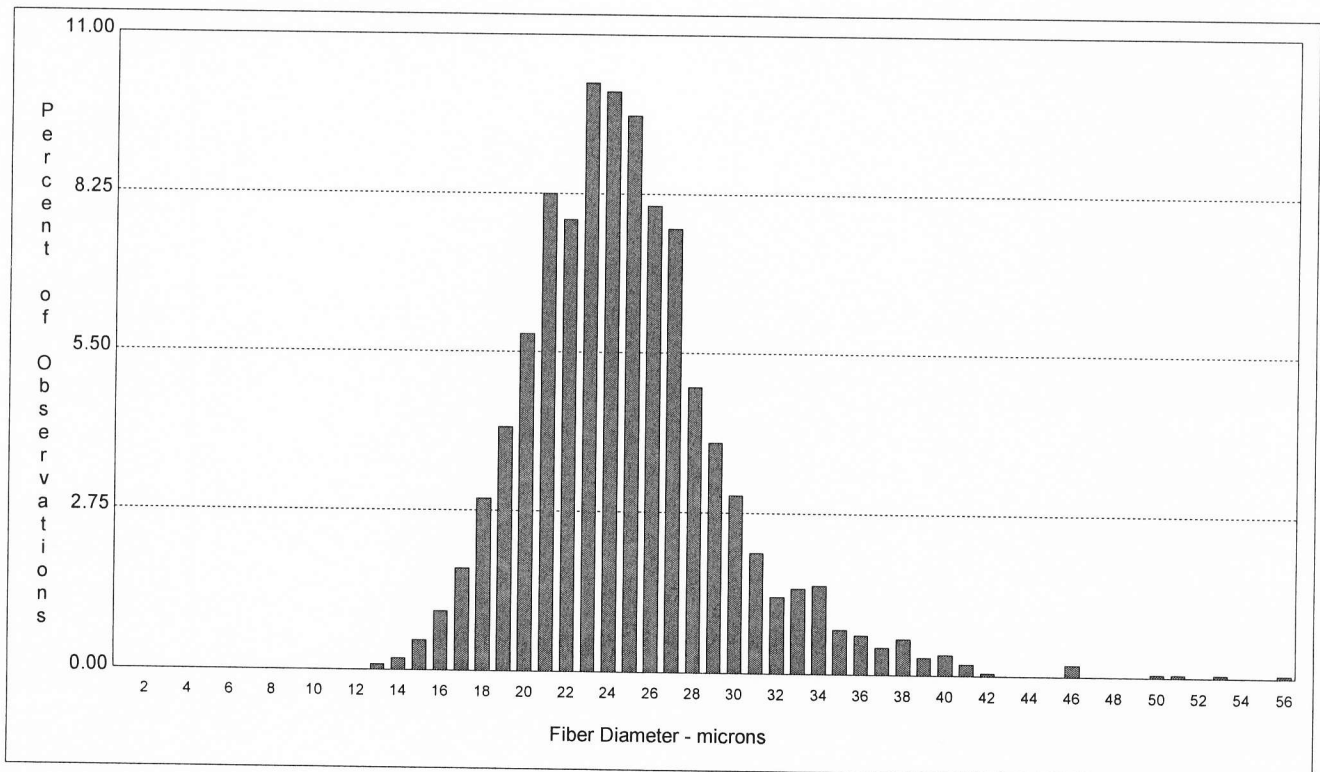

This Test Performed According to I.W.T.O Method 12