

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

R & R Ranch/Richard & Robin Vasquez
325B Denio Avenue
Gilroy CA 95020-9203 USA

07/19/10

Test No: 384079


Animal and Sample Description

Animal Name: Chela
Breed: Alpaca(Huacaya)
Sex: Female
Color: Appy

Animal ID: 814790
Sample Location: Side
Sample Date: 06/03/10
Age: 07/17/99

Laboratory Data

Mean Fiber Diameter: 35.4 microns
Standard Deviation: 6.4 microns
Coefficient of Variation: 18.2 %
Fibers Greater Than 30 microns: 78.0 %

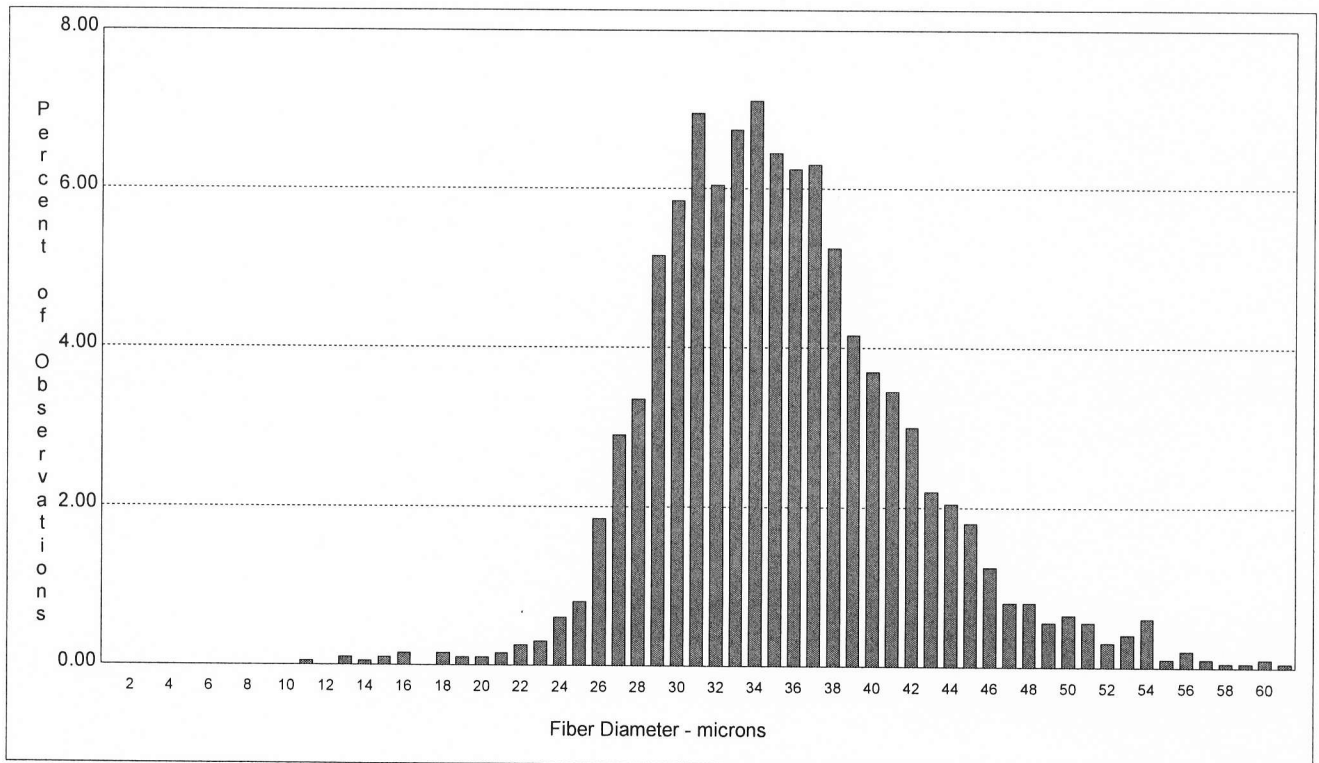

This Test Performed According to I.W.T.O Method 12