



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Diversified Alpacas LLC/Jennifer Schalk
1101 West Madison Road
St. Louis MI 48880 USA

Date: 09/28/12

Test No: 446027


Animal and Sample Description

Animal Name: Missy B
Breed: Alpaca(Huacaya)
Sex: Female
Color: Lt Fawn

Animal ID: 32209372
Sample Location: Side
Sample Date: 05/30/12
Age: 06/09/11

Laboratory Data

Mean Fiber Diameter:	18.5 microns	Fibers Greater Than 30 microns:	0.2 %
Standard Deviation:	3.2 microns	Comfort Factor:	99.8 %
Coefficient of Variation:	17.4 %	Mean Curvature:	45.8 deg/mm
Spin Fineness:	17.5 microns	SD Curvature:	24.5 deg/mm

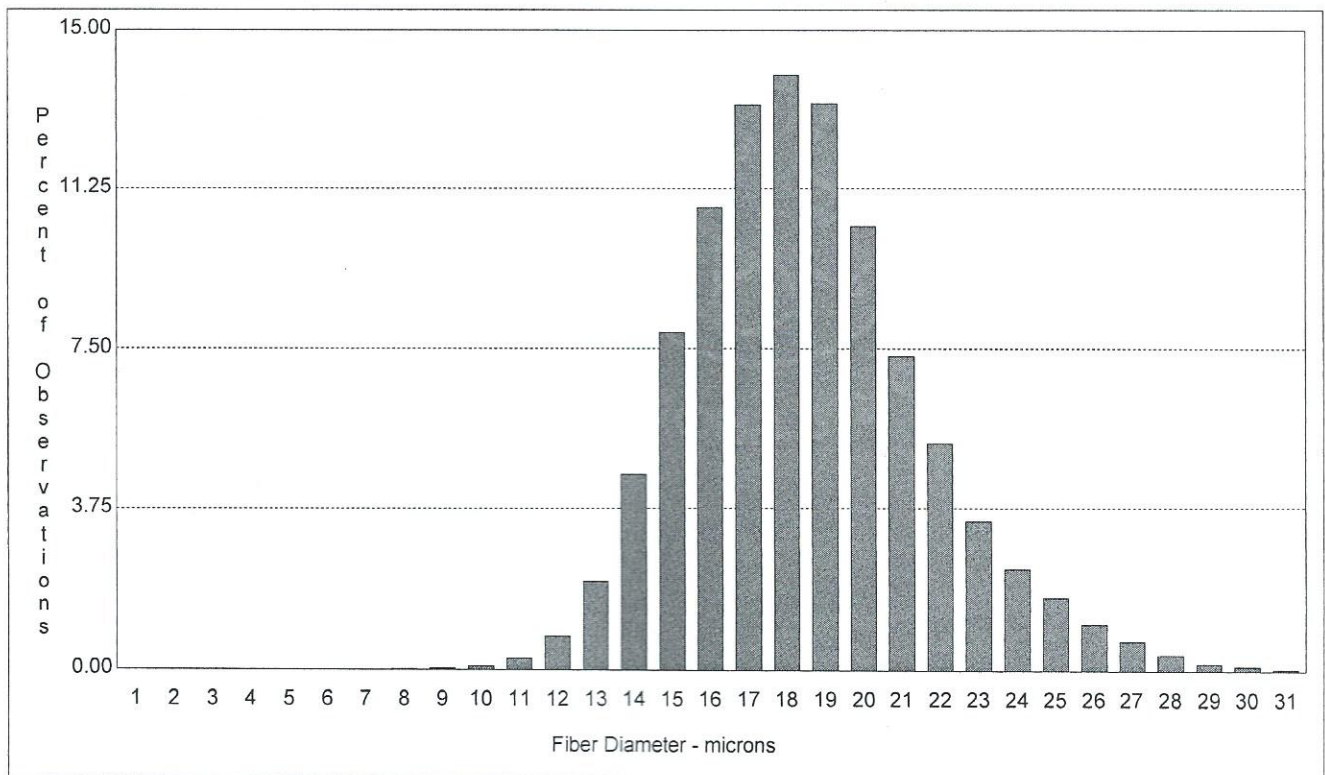

This Test Performed According to I.W.T.O Method 47