



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Xanadu Farm/Pamela Ray
669 Emerson Street
Denver CO 80218 USA

07/18/12

Test No: 435977


Animal and Sample Description

Animal Name: Counter Point
Breed: Alpaca(Huacaya)
Sex: XXXXX
Color: XXXXX

Animal ID: XXXXX
Sample Location: Side
Sample Date: 04/27/12
Age: XXXXX

Laboratory Data

| | | | |
|--|--------------|---------------------------------|--------------|
| Mean Fiber Diameter: | 16.7 microns | Spin Fineness: | 17.4 microns |
| Standard Deviation: | 4.7 microns | Mean Curvature (deg/mm): | 53.9 |
| Coefficient of Variation: | 28.0 % | SD Curvature (deg/mm): | 25.4 |
| Fibers Greater Than 30 microns: | 1.0 % | Comfort Factor: | 99.0 % |
| Medullated Fibers: | 8.6 % | | |

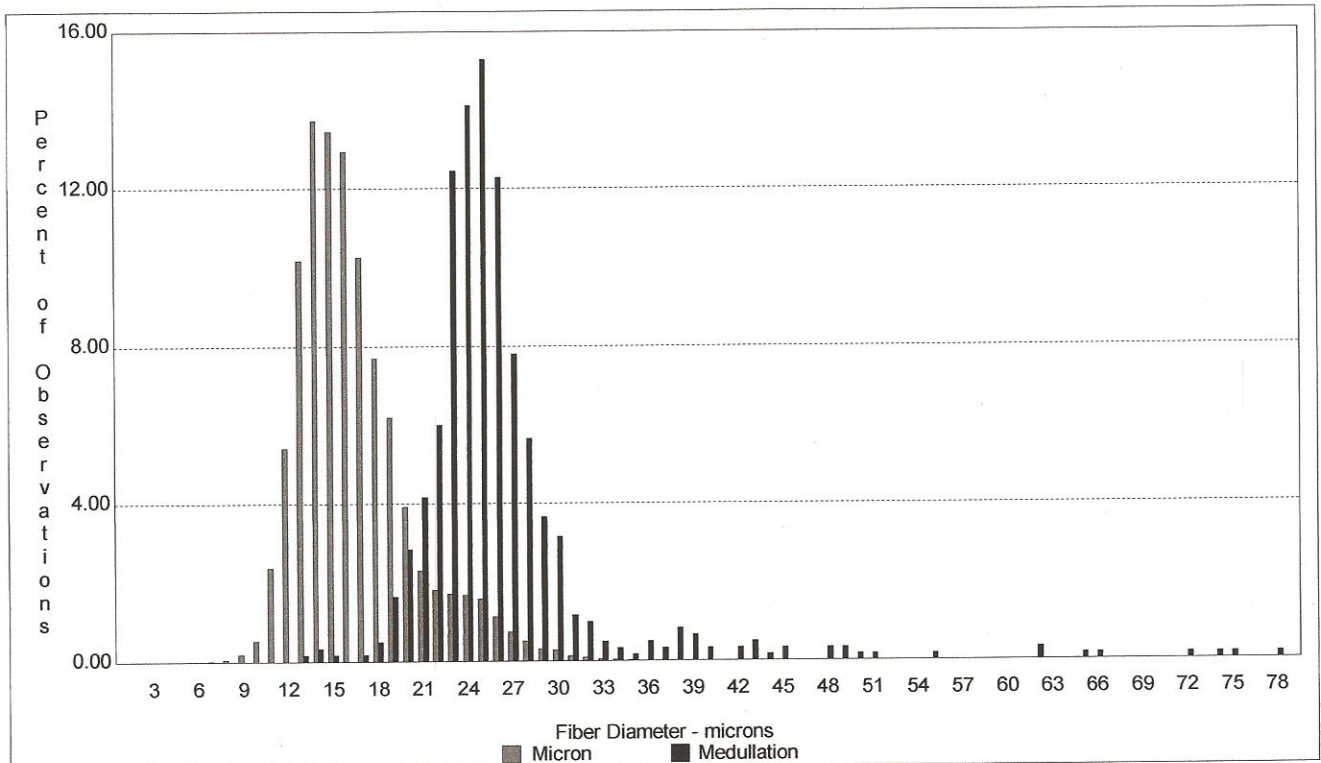

This Test Performed According to I.W.T.O Method 47