

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan
Micron Test Report

Owl Ridge Alpacas/Jodie & Dan Vanselow
7842 Hall Rd
Interlaken NY 14847 USA

05/30/13

Test No: 454587


Animal and Sample Description

Animal Name: Owl Ridge Pixie Twix
Breed: Alpaca(Huacaya)
Sex: Female
Color: Lt Brown

Animal ID: XXXXX
Sample Location: Side
Sample Date: 05/03/13
Age: 05/26/12

Laboratory Data

Mean Fiber Diameter: 16.5 microns
Standard Deviation: 3.2 microns
Coefficient of Variation: 19.5 %
Fibers Greater Than 30 microns: 0.7 %

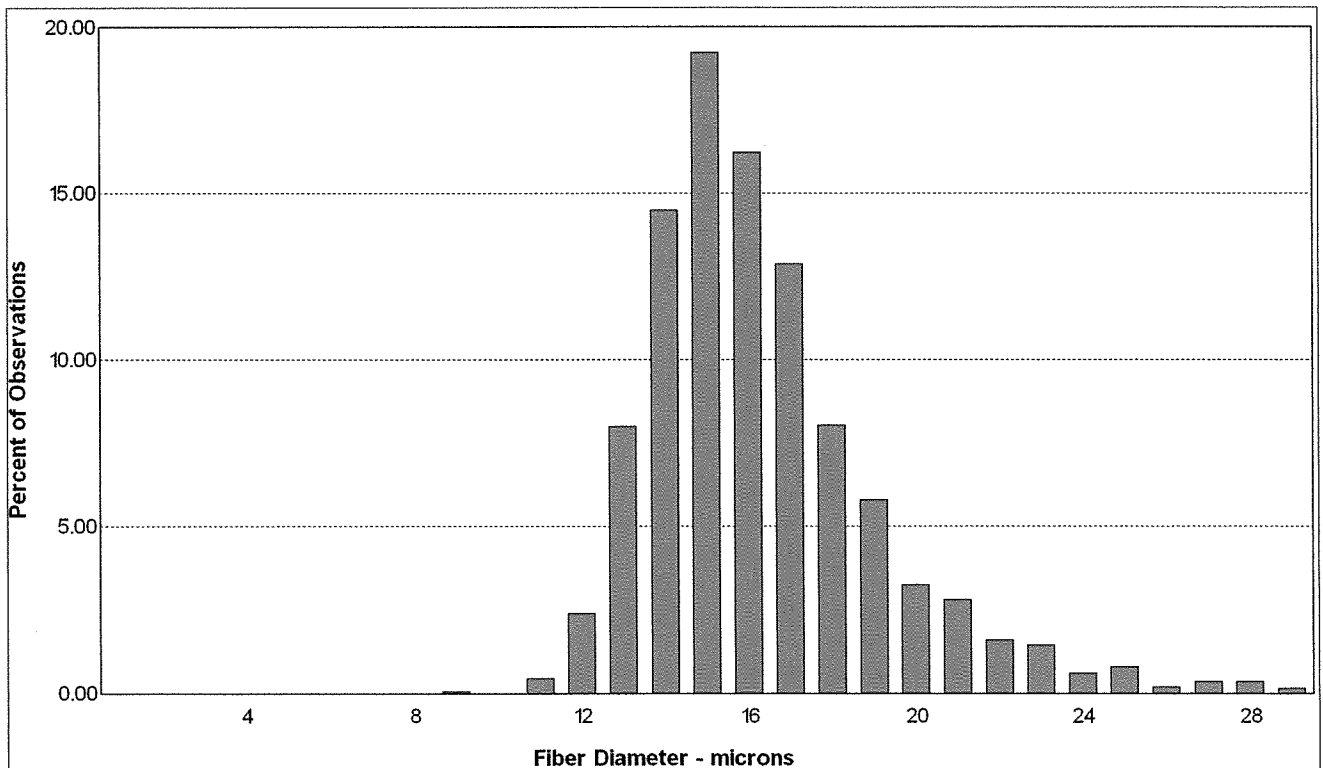

This Test Performed According to I.W.T.O Method 12