



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

The Wood Farm/Libby Stover
14 Wood Road
Franklin PA 16323 U.S.A

06/26/14

Test No: 482620


Animal and Sample Description

Animal Name: TWF Peruvian Chantilly Lace
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 32484458
Sample Location: Mid Side
Sample Date: 05/23/14
Age: 07/14/12

Laboratory Data

Mean Fiber Diameter: 15.6 microns
Standard Deviation: 3.2 microns
Coefficient of Variation: 20.6 %
Fibers Greater Than 30 microns: 0.4 %

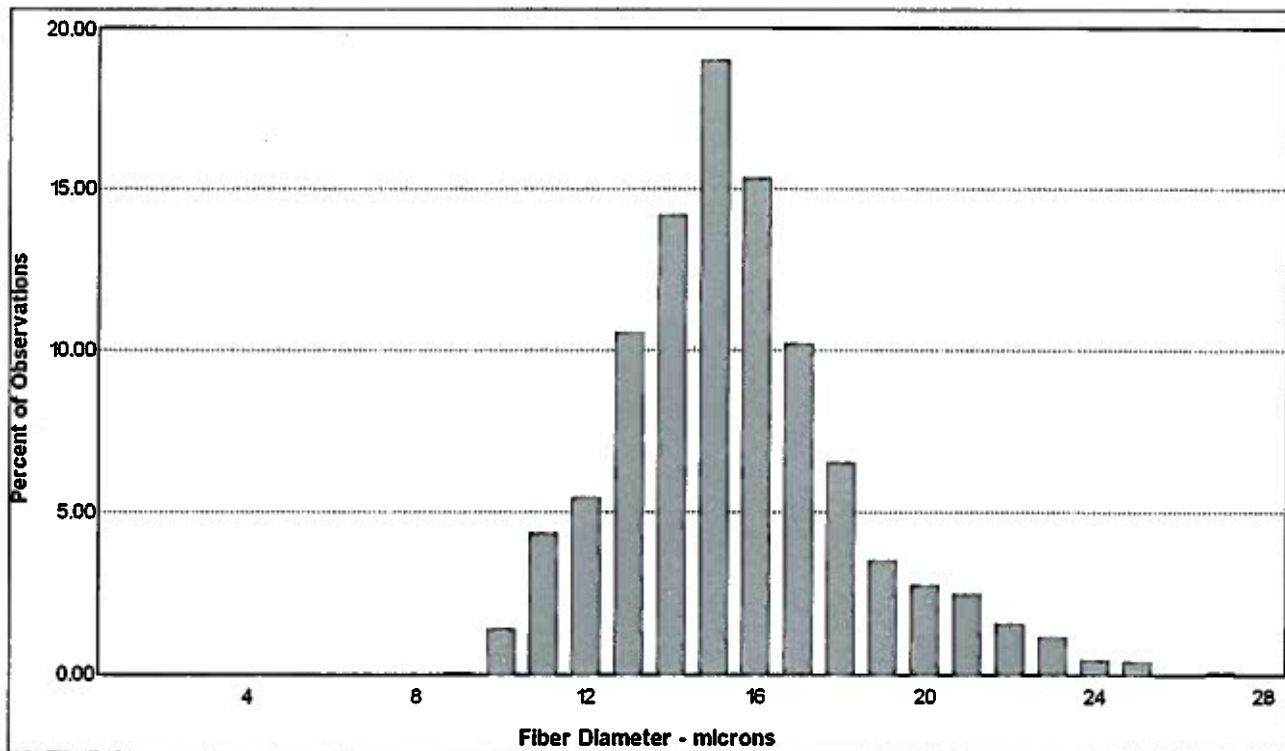

This Test Performed According to I.W.T.O Method 12