



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Good Karma Ranch, LLC/Michael Walsh
1041 Brevard Place Rd
Iron Station NC 28080 USA

Date: 09/08/14

Test No: 492210


Animal and Sample Description

Animal Name: Snowmass Matrix Moon
Breed: Alpaca(Huacaya)
Sex: Male
Color: Beige

Animal ID: 31778862
Sample Location: Side
Sample Date: 04/26/14
Age: 04/25/10

Laboratory Data

Mean Fiber Diameter:	17.8 microns	Fibers Greater Than 30 microns:	0.5 %
Standard Deviation:	3.6 microns	Comfort Factor:	99.5 %
Coefficient of Variation:	20.0 %	Mean Curvature:	55.2 deg/mm
Spin Fineness:	17.2 microns	SD Curvature:	28.1 deg/mm

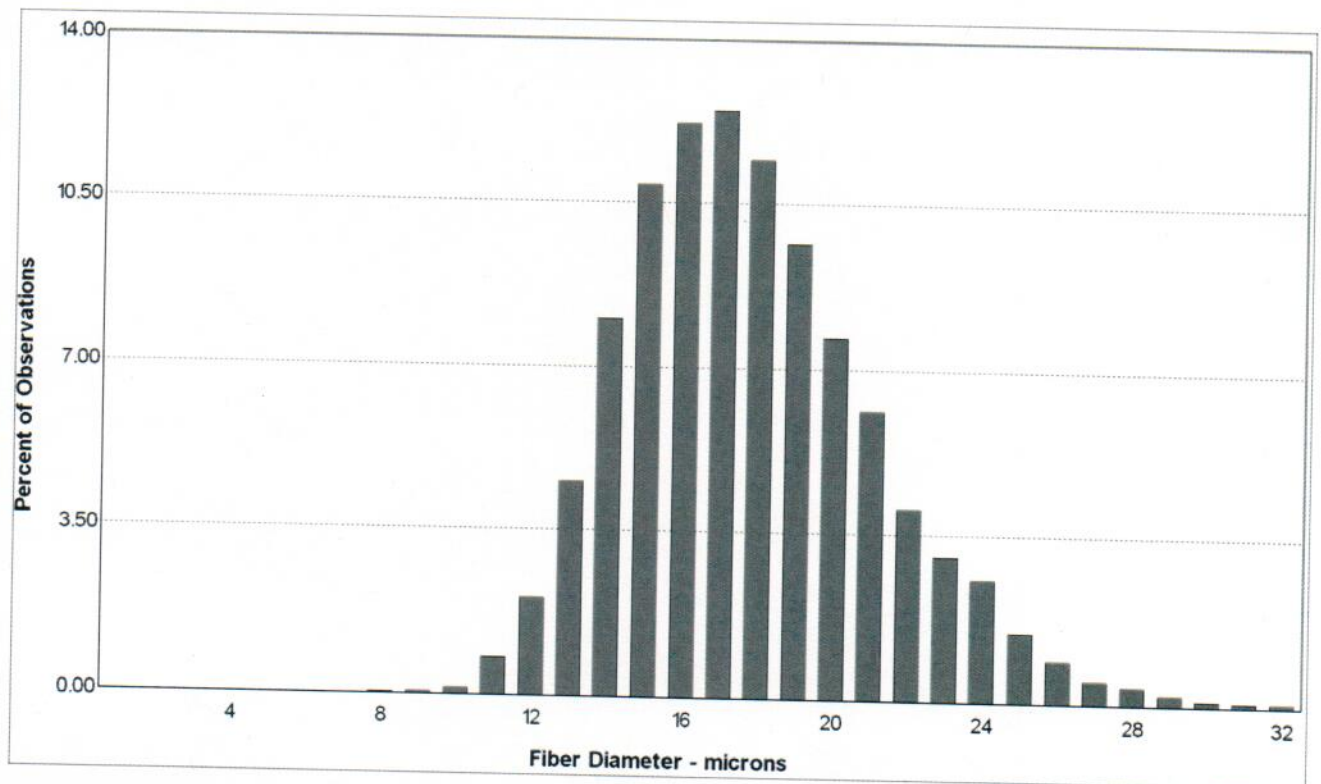

This Test Performed According to I.W.T.O Method 47