



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

OakHill Alpacas, LLC/Joyce Calderwood  
7226 First Avenue  
Mays Landing NJ 08330 USA

08/05/14

Test No: 488899


### Animal and Sample Description

**Animal Name:** NJOakhill's Sandstorm  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** Lt Fawn

**Animal ID:** 32687019  
**Sample Location:** Side  
**Sample Date:** 05/08/14  
**Age:** 06/19/11

### Laboratory Data

**Mean Fiber Diameter:** 18.6 microns  
**Standard Deviation:** 4.1 microns  
**Coefficient of Variation:** 21.9 %  
**Fibers Greater Than 30 microns:** 1.2 %

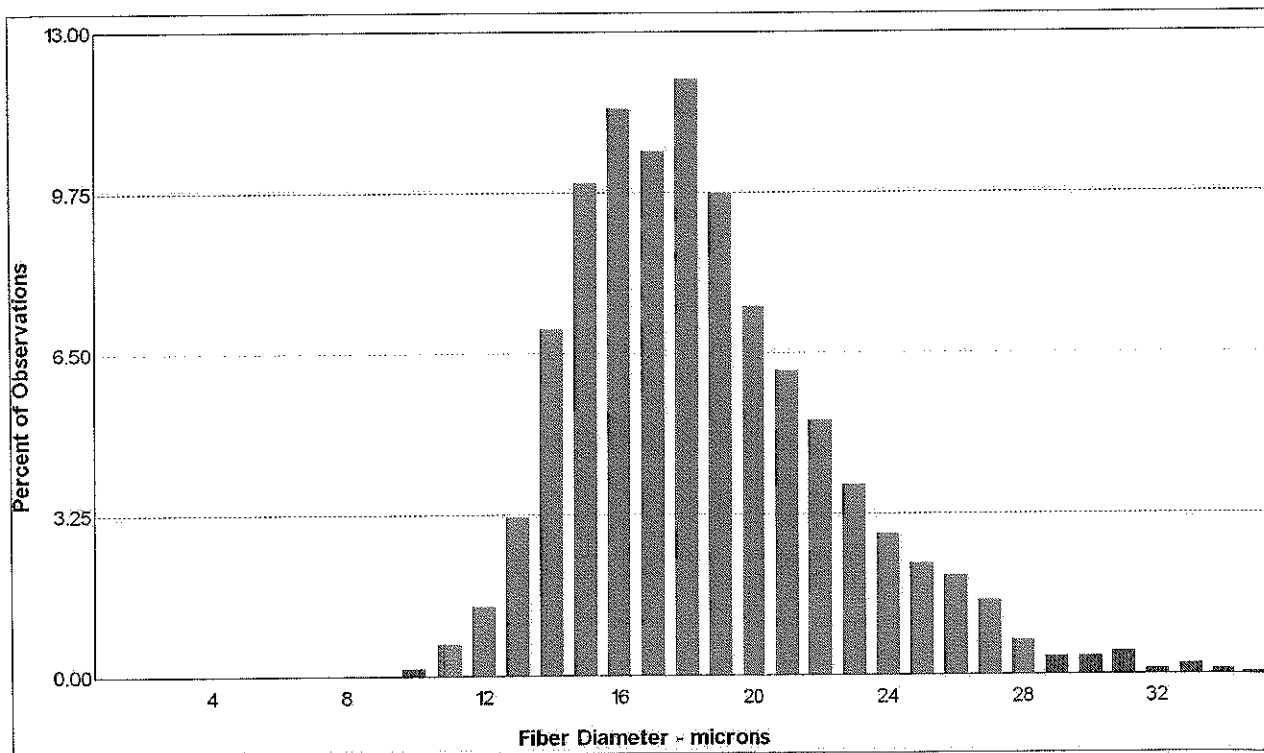

This Test Performed According to I.W.T.O Method 12