



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Tripping Gnome Farm/Ursula Munro
64 Lupine Lane
Freeport ME 04032

06/28/13

Test No: 457106


Animal and Sample Description

Animal Name: TGF Supreme Summit
Breed: Alpaca(Huacaya)
Sex: Male
Color: WH

Animal ID: 32097764
Sample Location: Side (R)
Sample Date: 05/10/13
Age: 09/19/10

Laboratory Data

Mean Fiber Diameter:	20.9 microns	Spin Fineness:	19.9 microns
Standard Deviation:	3.9 microns	Mean Curvature (deg/mm):	48.6
Coefficient of Variation:	18.7 %	SD Curvature (deg/mm):	24.9
Fibers Greater Than 30 microns:	2.2 %	Comfort Factor:	97.8 %
Medullated Fibers:	4.0 %		

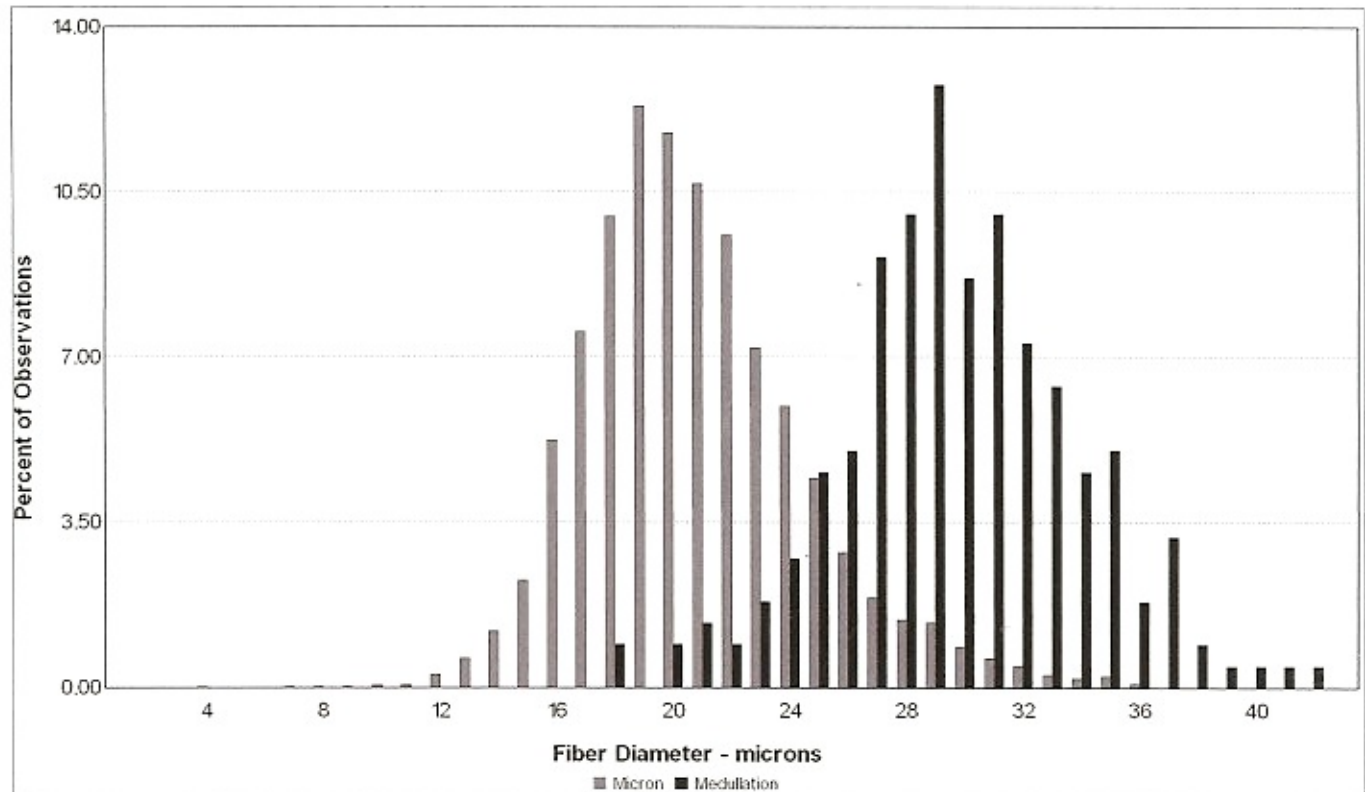

This Test Performed According to I.W.T.O Method 47